
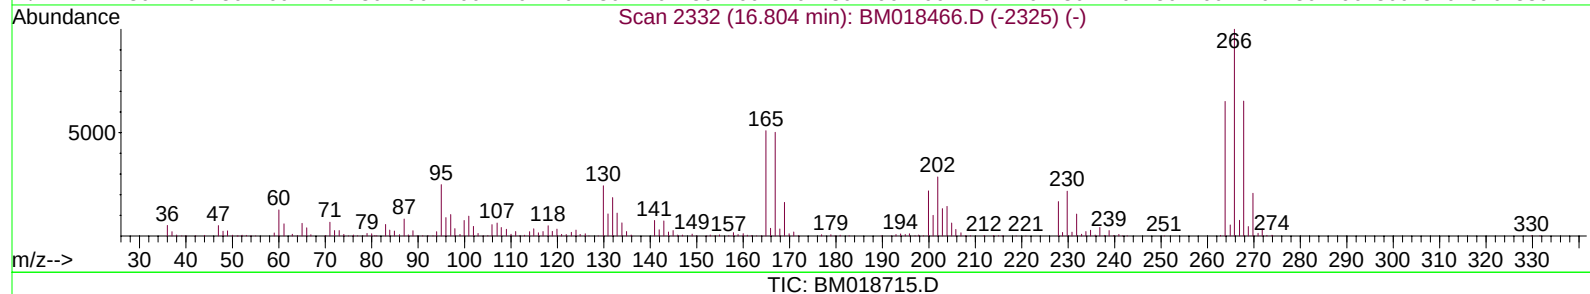
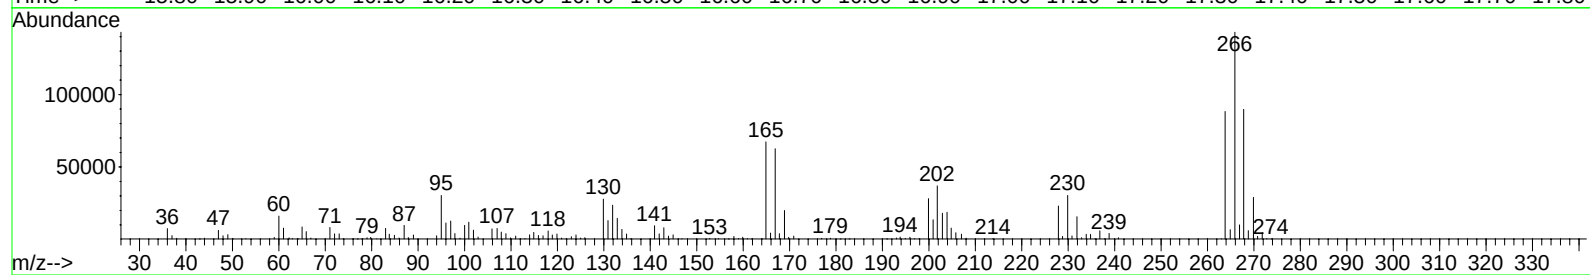


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM020419\
Data File : BM018715.D
Acq On : 04 Feb 2019 12:59
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 18:06:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 04 15:10:38 2019
Response via : Initial Calibration

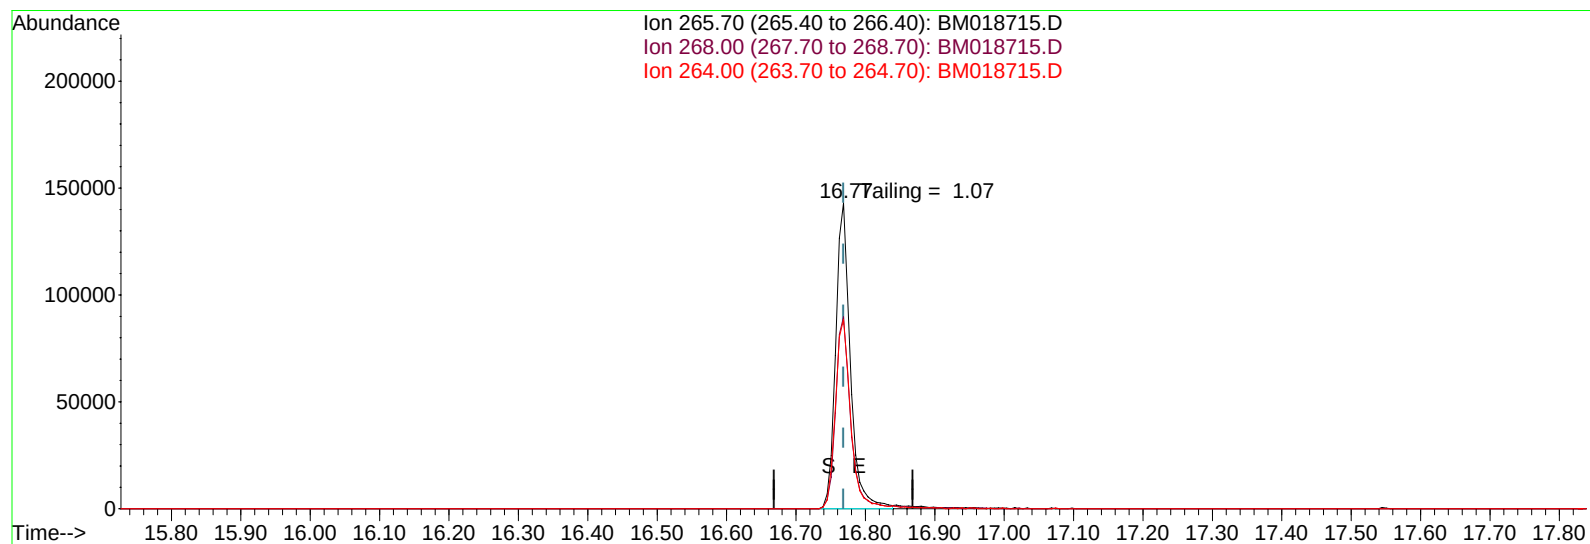

(70) Pentachlorophenol (C)




16.768min (+0.000) 38578.81ng

response 209857

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.74
264.00	62.60	61.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM020419\
 Data File : BM018715.D
 Acq On : 04 Feb 2019 12:59
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 18:06:09 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 04 15:10:38 2019
 Response via : Initial Calibration

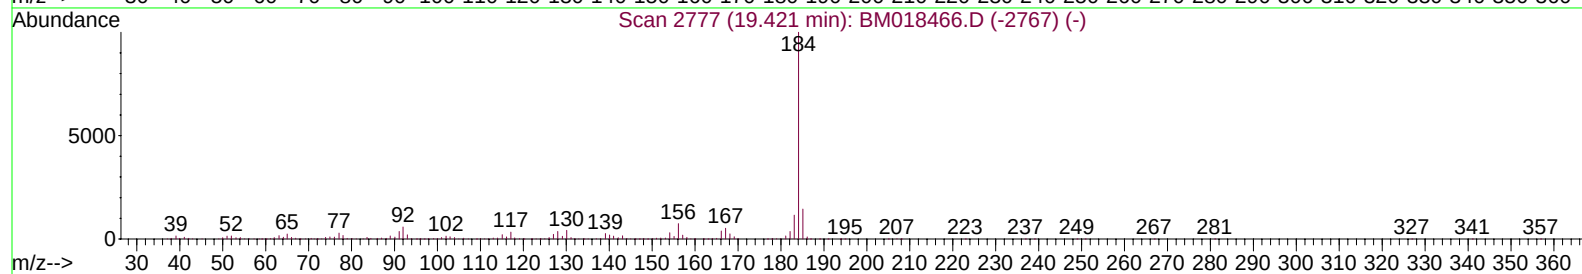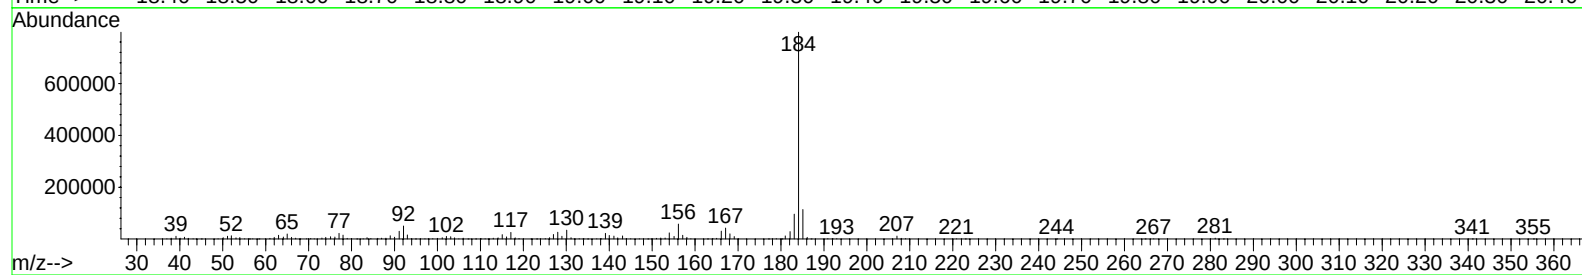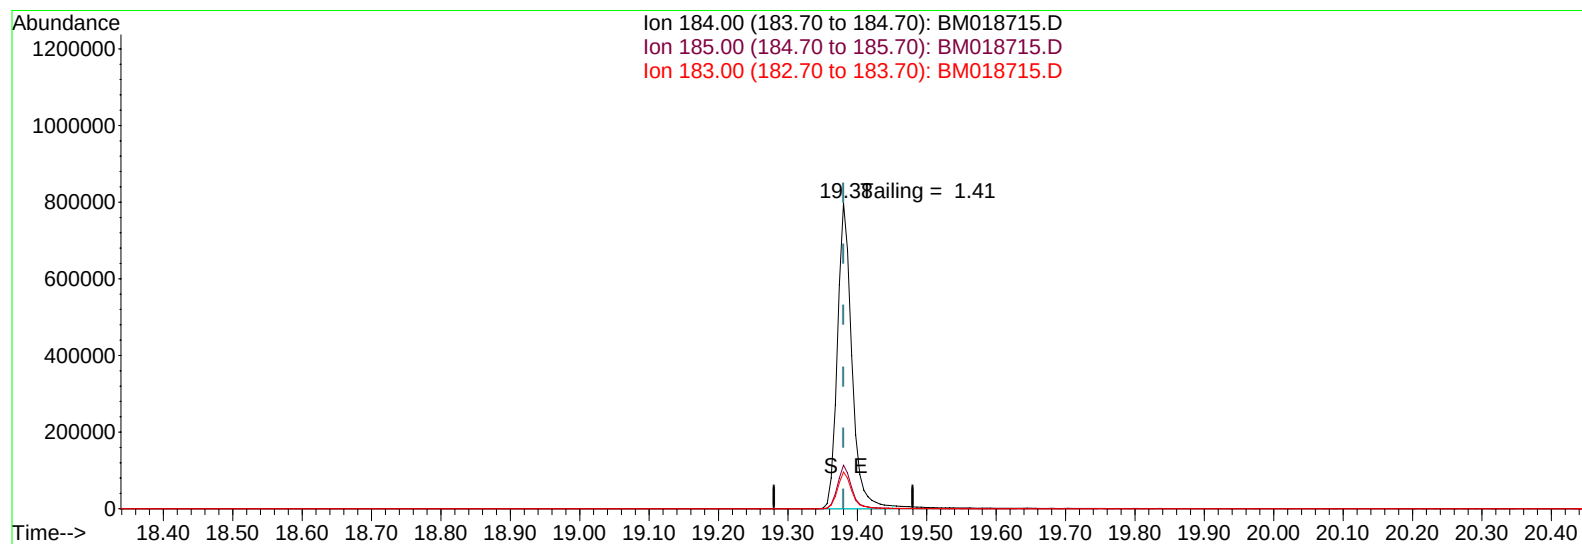

TIC: BM018715.D

(77) Benzidine

19.380min (+0.000) 48462.01ng

response 1151127

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.30
183.00	11.90	12.03
0.00	0.00	0.00