


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM020419\
 Data File : BM018715.D
 Acq On : 04 Feb 2019 12:59
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 04 15:10:38 2019

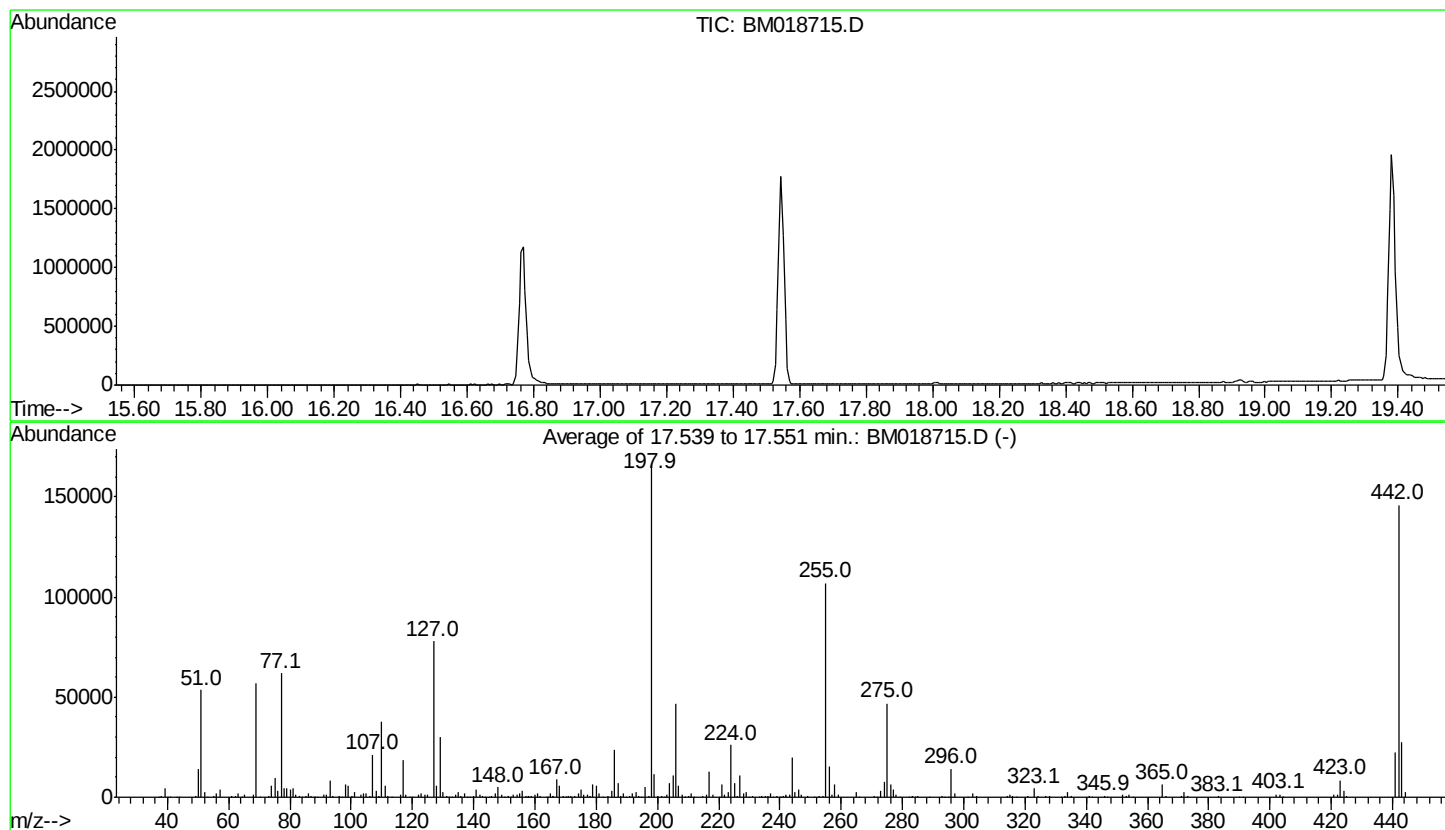

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	53448	PASS
68	69	0.00	2	1.9	1106	PASS
69	198	0.00	100	34.5	57194	PASS
70	69	0.00	2	0.3	147	PASS
127	198	10	80	47.1	77949	PASS
197	198	0.00	2	0.5	895	PASS
198	198	100	100	100.0	165568	PASS
199	198	5	9	7.2	11847	PASS
275	198	10	60	28.3	46912	PASS
365	198	1	100	3.7	6188	PASS
441	198	0.01	100	13.4	22223	PASS
442	198	50	100	88.1	145789	PASS
443	442	15	24	18.8	27429	PASS