


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM020719\
 Data File : BM018732.D
 Acq On : 07 Feb 2019 11:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 04 15:10:38 2019

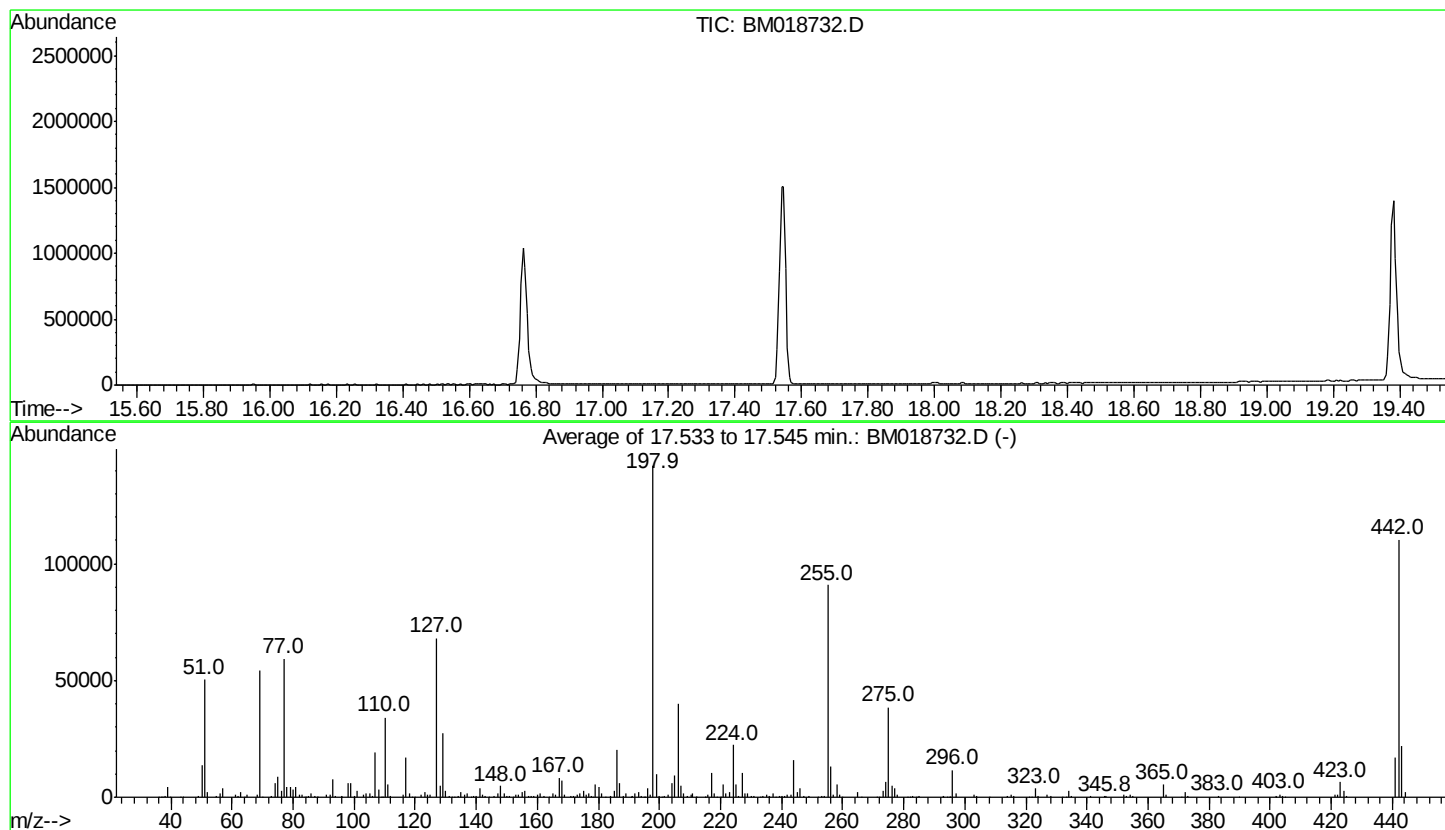

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	50194	PASS
68	69	0.00	2	2.0	1063	PASS
69	198	0.00	100	38.3	54362	PASS
70	69	0.00	2	0.5	246	PASS
127	198	10	80	48.0	68173	PASS
197	198	0.00	2	0.6	843	PASS
198	198	100	100	100.0	142026	PASS
199	198	5	9	6.8	9717	PASS
275	198	10	60	27.1	38509	PASS
365	198	1	100	3.8	5405	PASS
441	198	0.01	100	11.9	16843	PASS
442	198	50	100	77.6	110253	PASS
443	442	15	24	19.7	21709	PASS