



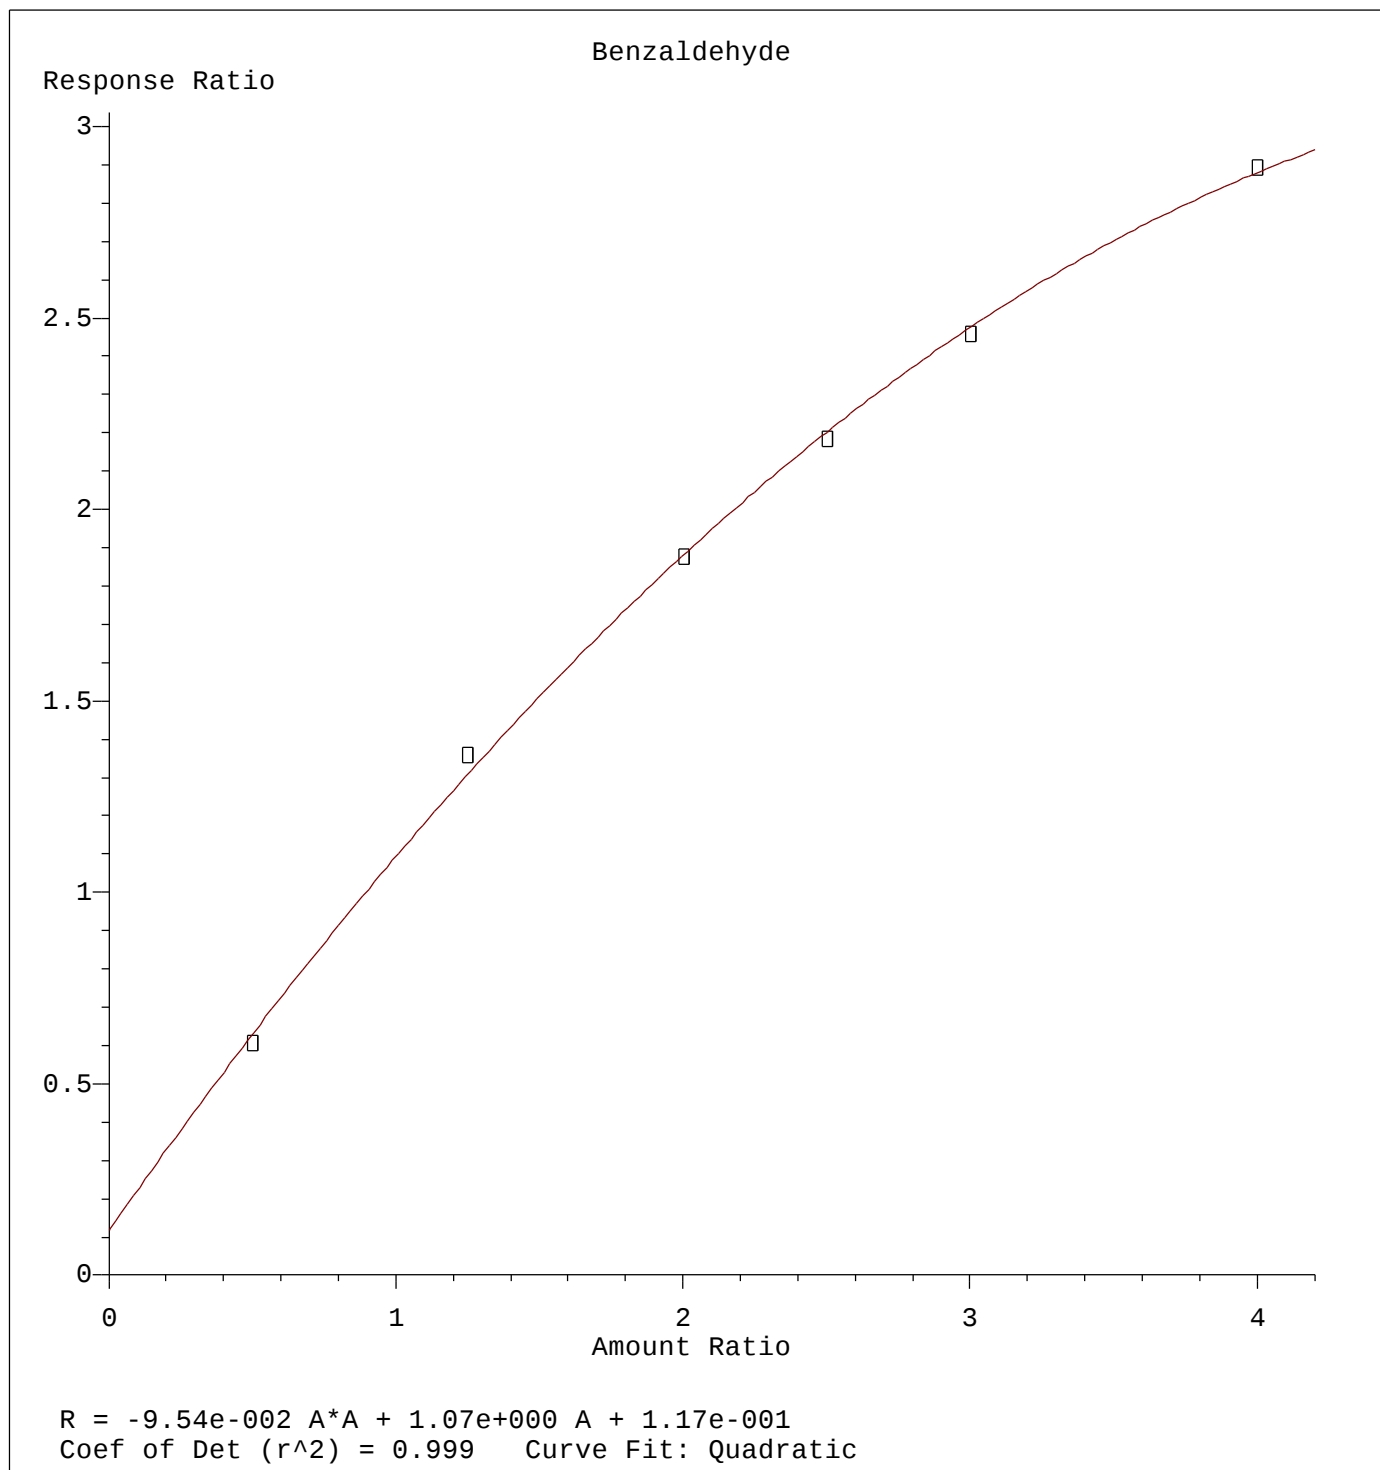

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Calibration Table Last Updated: Mon Feb 11 16:02:12 2019

2,4-Dinitrophenol

Response Ratio

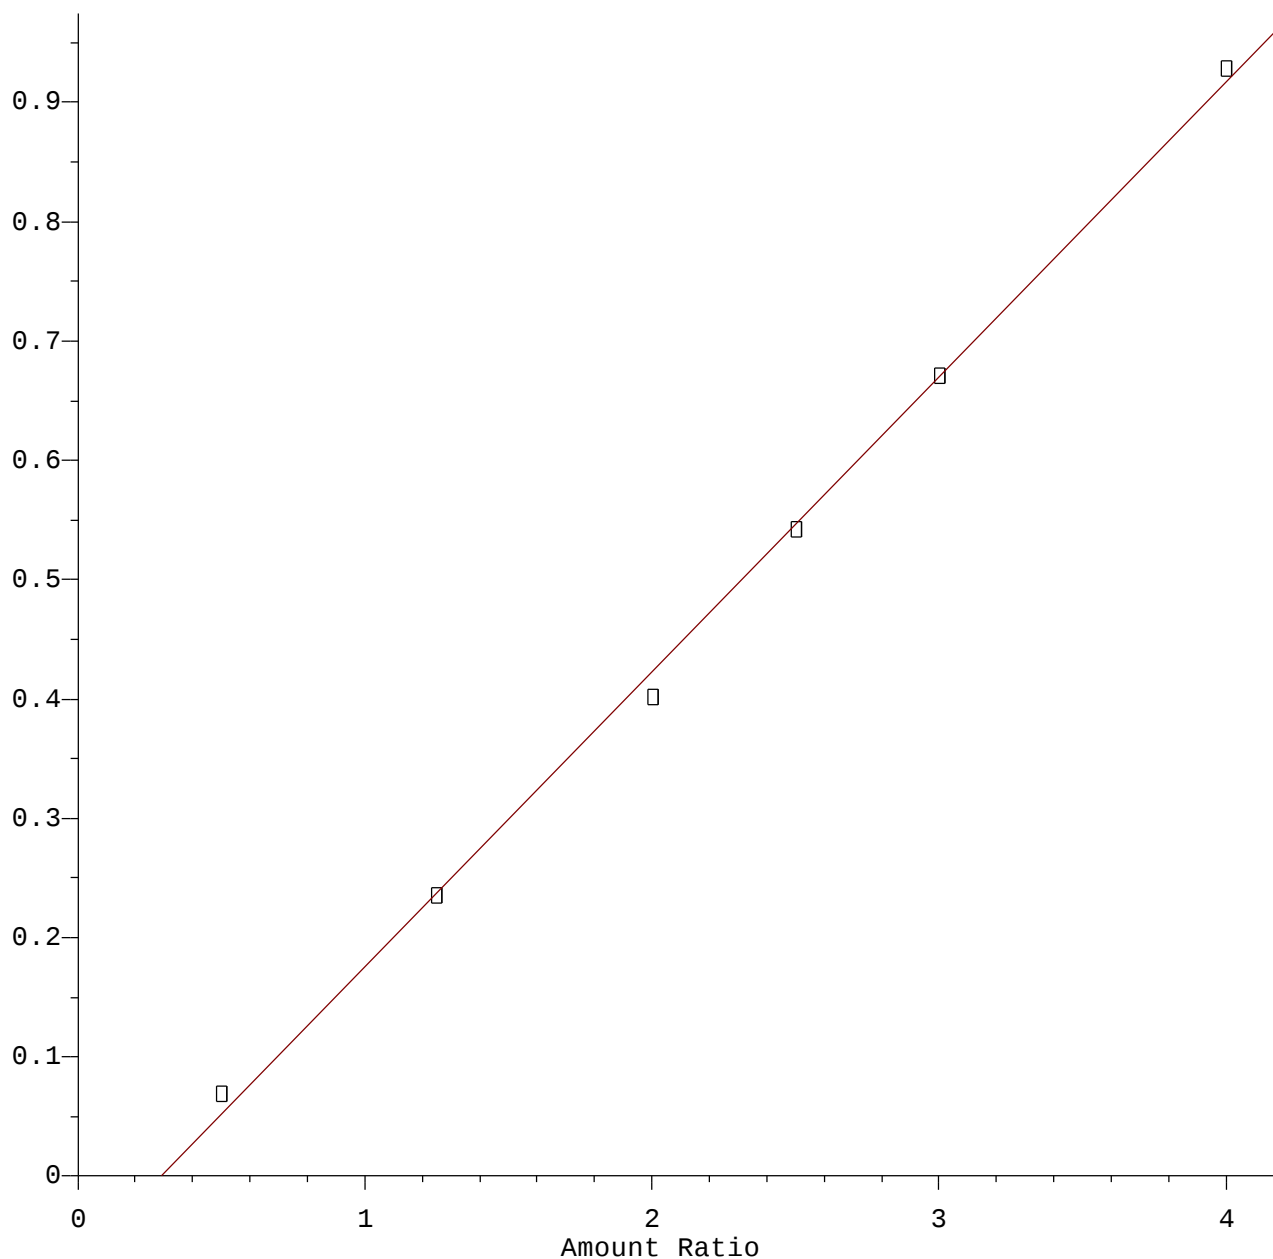

Resp Ratio = 2.47e-001 * Amt - 7.11e-002
Coef of Det (r²) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Calibration Table Last Updated: Mon Feb 11 16:02:12 2019