
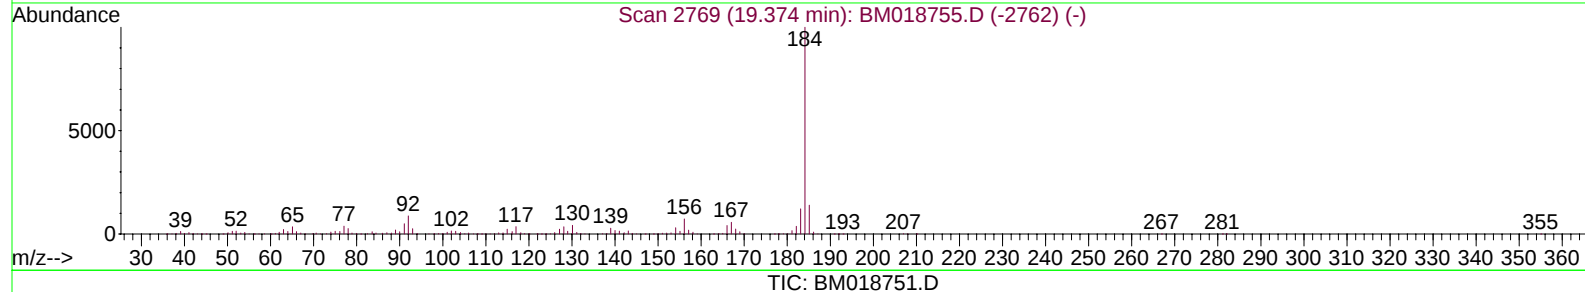
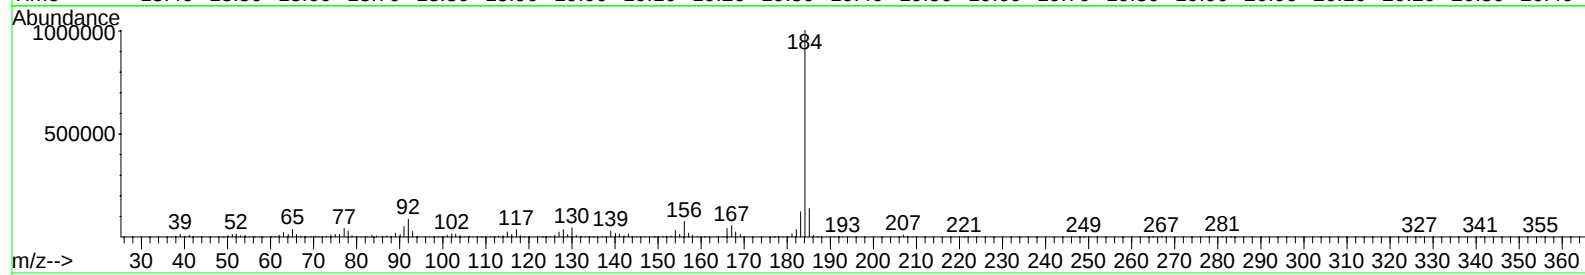


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021119\
Data File : BM018751.D
Acq On : 11 Feb 2019 10:58
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 18:20:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

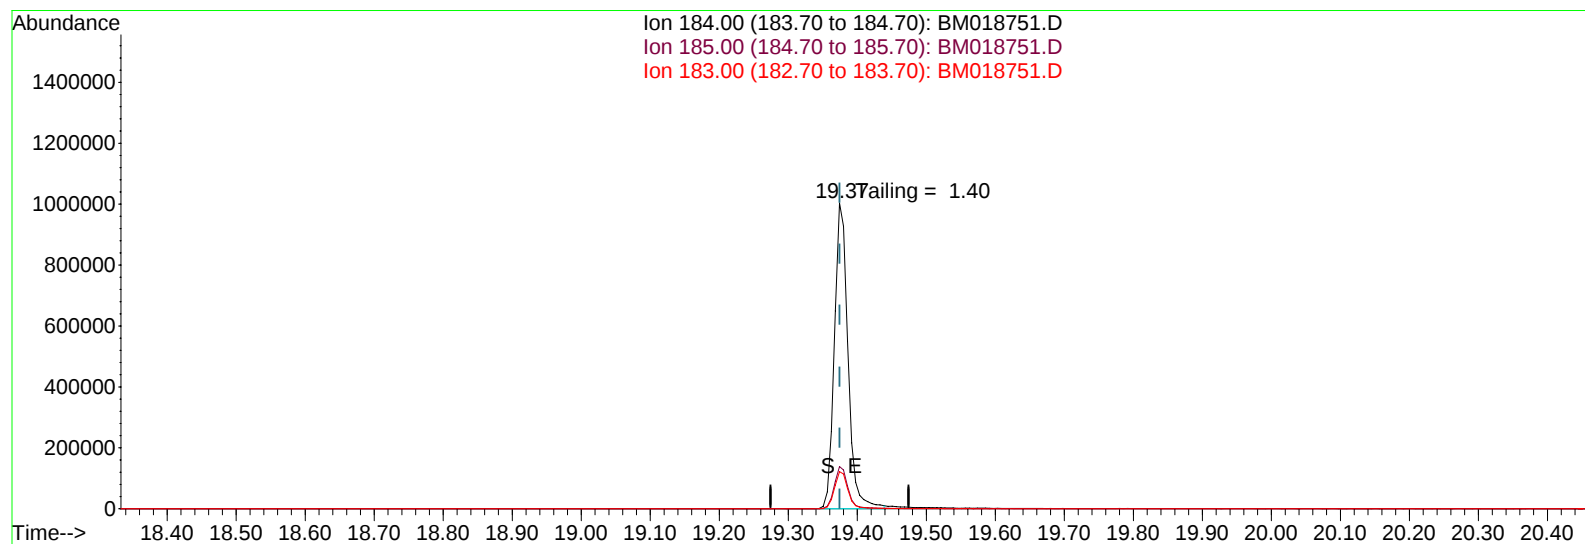

(77) Benzidine




19.374min (-0.000) 78108.21ng

response 1386177

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.81
183.00	12.10	12.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021119\
Data File : BM018751.D
Acq On : 11 Feb 2019 10:58
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 18:20:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

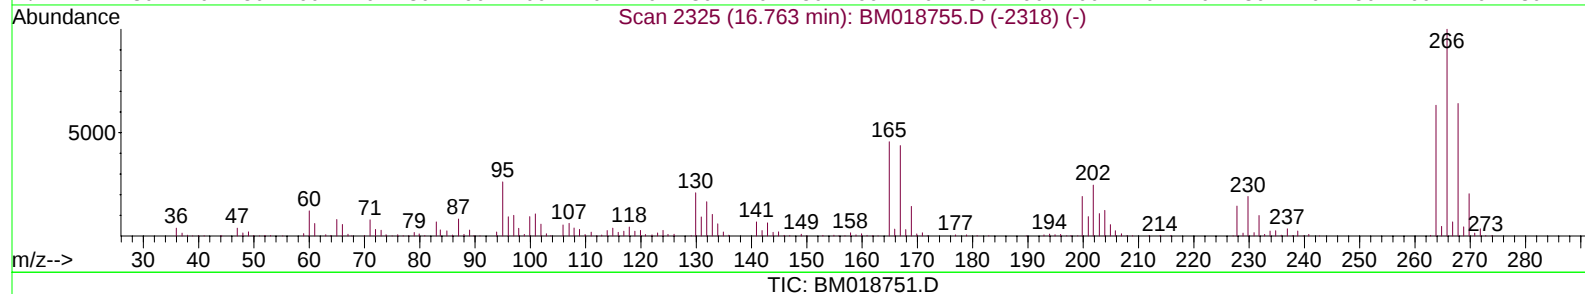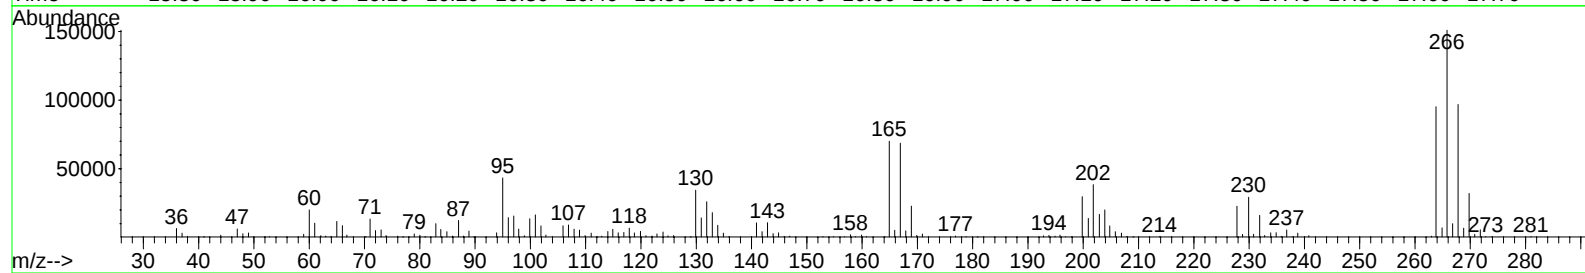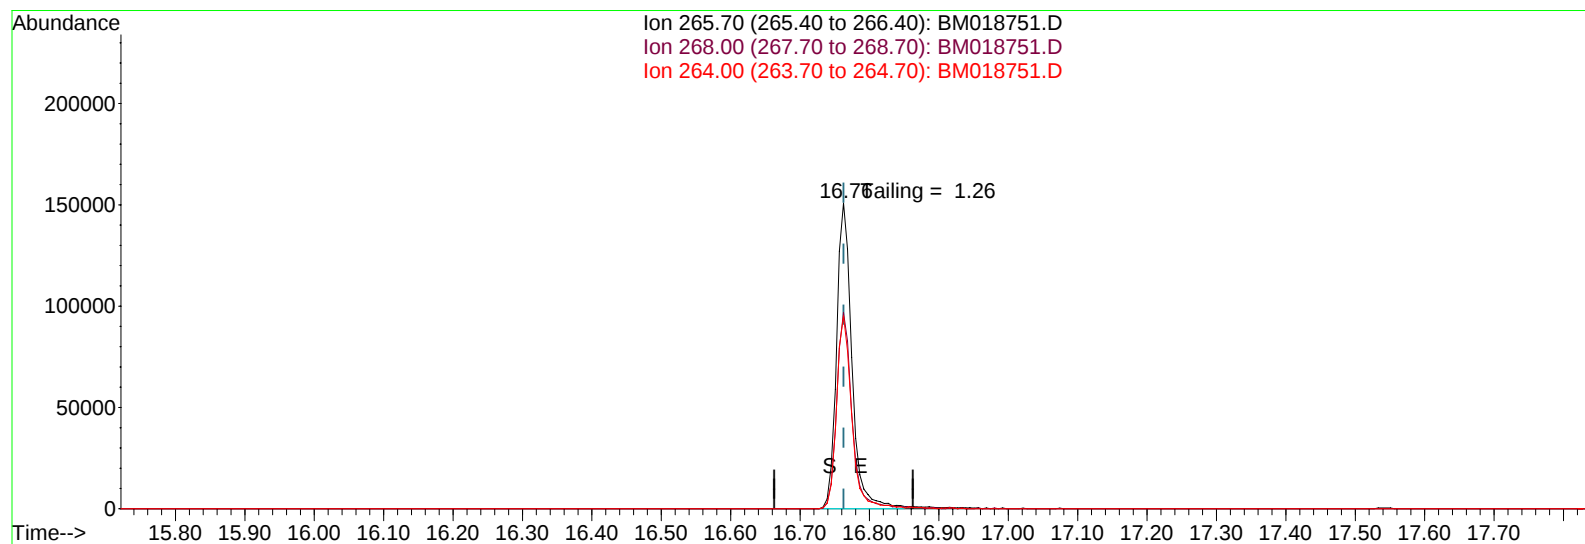

(70) Pentachlorophenol (C)

16.762min (-0.000) 46806.78ng

response 230560

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	64.13
264.00	63.20	63.06
0.00	0.00	0.00