

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021119\
 Data File : BM018763.D
 Acq On : 11 Feb 2019 18:29
 Operator : JU/SJ
 Sample : K1404-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FB-02-06-19

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.304	371	377	395	rBV	2330769	3405375	14.49%	3.495%
2	6.887	639	646	658	rBV	1259475	2051423	8.73%	2.106%
3	7.245	700	707	726	rBV	4895139	7640214	32.52%	7.842%
4	7.716	780	787	793	rBV	1090590	1747389	7.44%	1.793%
5	8.028	833	840	854	rBV	4526259	7259625	30.90%	7.451%
6	8.881	977	985	1001	rBV	3656009	5955065	25.35%	6.112%
7	10.504	1253	1261	1272	rBV	1326816	2300429	9.79%	2.361%
8	12.980	1674	1682	1699	rBV	9419317	13637263	58.04%	13.997%
9	14.363	1906	1917	1934	rBV2	2004127	3108877	13.23%	3.191%
10	15.857	2164	2171	2194	rBV	7622680	10956158	46.63%	11.245%
11	17.115	2378	2385	2398	rBV2	2672193	3884357	16.53%	3.987%
12	19.751	2826	2833	2838	rBV	18754501	23495145	100.00%	24.115%
13	20.374	2935	2939	2943	rBV	469235	499478	2.13%	0.513%
14	21.303	3092	3097	3104	rBV	4185727	5002626	21.29%	5.135%
15	22.345	3270	3274	3280	rVB	278172	371358	1.58%	0.381%
16	22.850	3356	3360	3367	rVB	314379	455650	1.94%	0.468%
17	23.421	3453	3457	3464	rVB	302701	469748	2.00%	0.482%
18	23.568	3475	3482	3492	rVB2	2431778	4770595	20.30%	4.896%
19	24.074	3564	3568	3575	rVB2	227921	419232	1.78%	0.430%


Sum of corrected areas: 97430007

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021119\
Data File : BM018763.D
Acq On : 11 Feb 2019 18:29
Operator : JU/SJ
Sample : K1404-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB-02-06-19

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

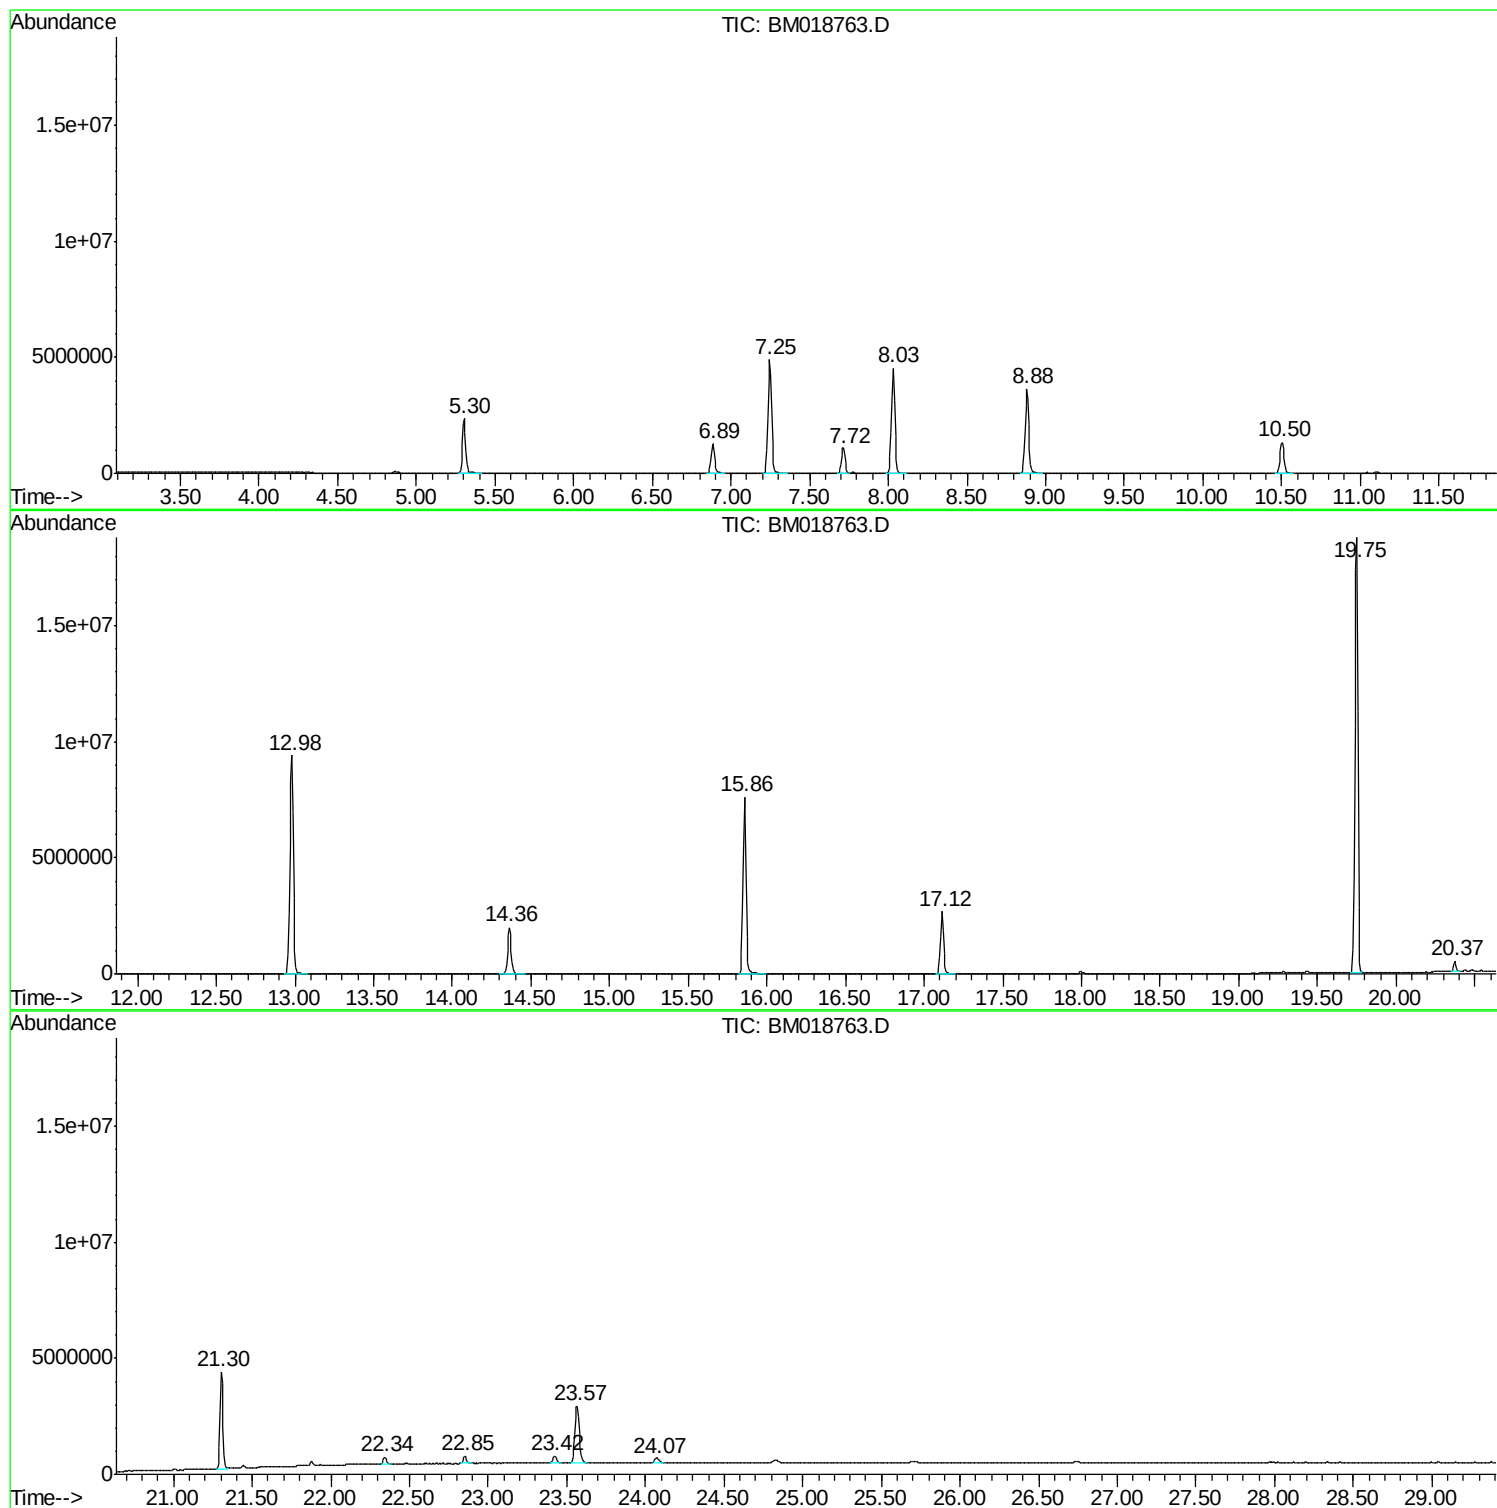

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021119\
Data File : BM018763.D
Acq On : 11 Feb 2019 18:29
Operator : JU/SJ
Sample : K1404-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB-02-06-19










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.25 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.25	87.45 ng	7640210	1,4-Dichlorobenzene-d4	7.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		2-Cyclohexen-1-one	96	C6H8O	000930-68-7	11
4		(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

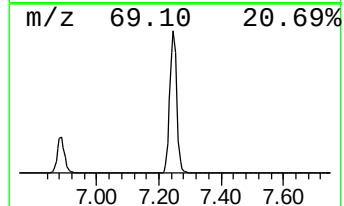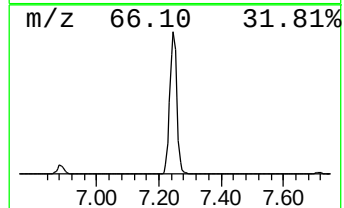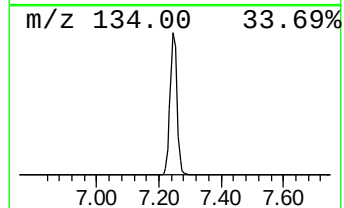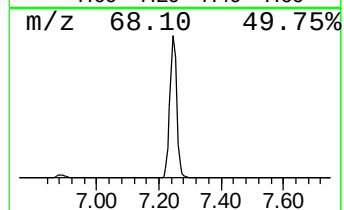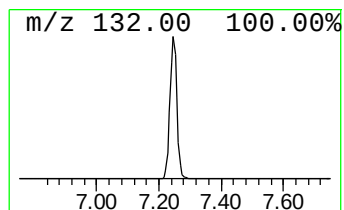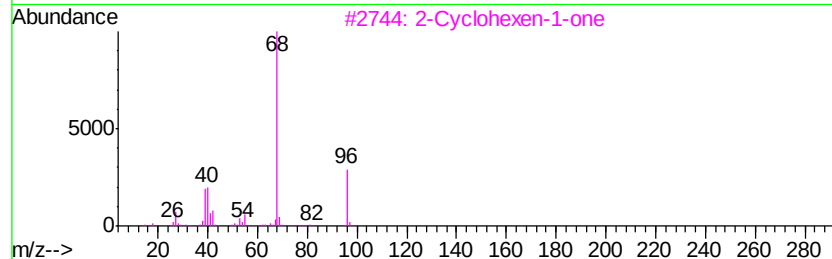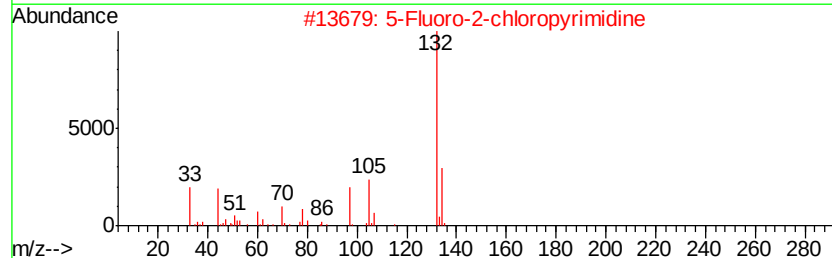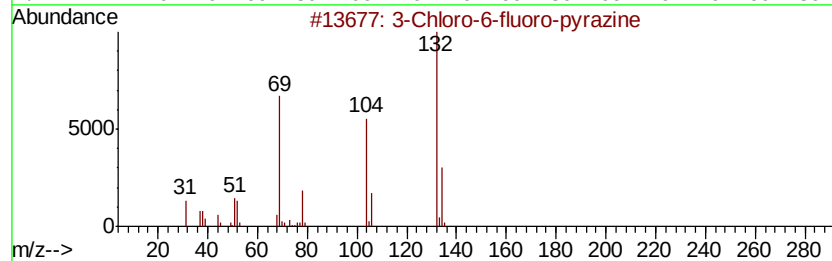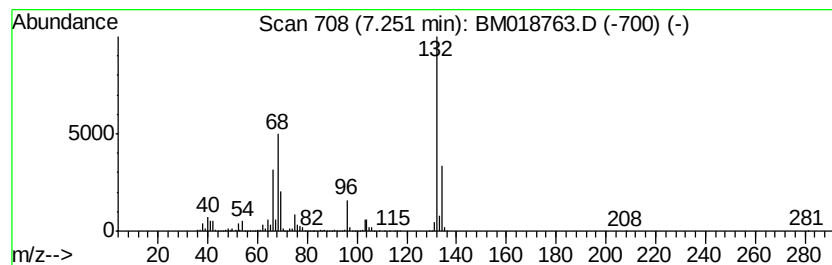

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM021119\
Data File : BM018763.D
Acq On : 11 Feb 2019 18:29
Operator : JU/SJ
Sample : K1404-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB-02-06-19

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.25	7.25	87.5	ng	7640210	1	7.72	1747390	20.0