


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021119\
 Data File : BM018751.D
 Acq On : 11 Feb 2019 10:58
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 11 16:02:12 2019

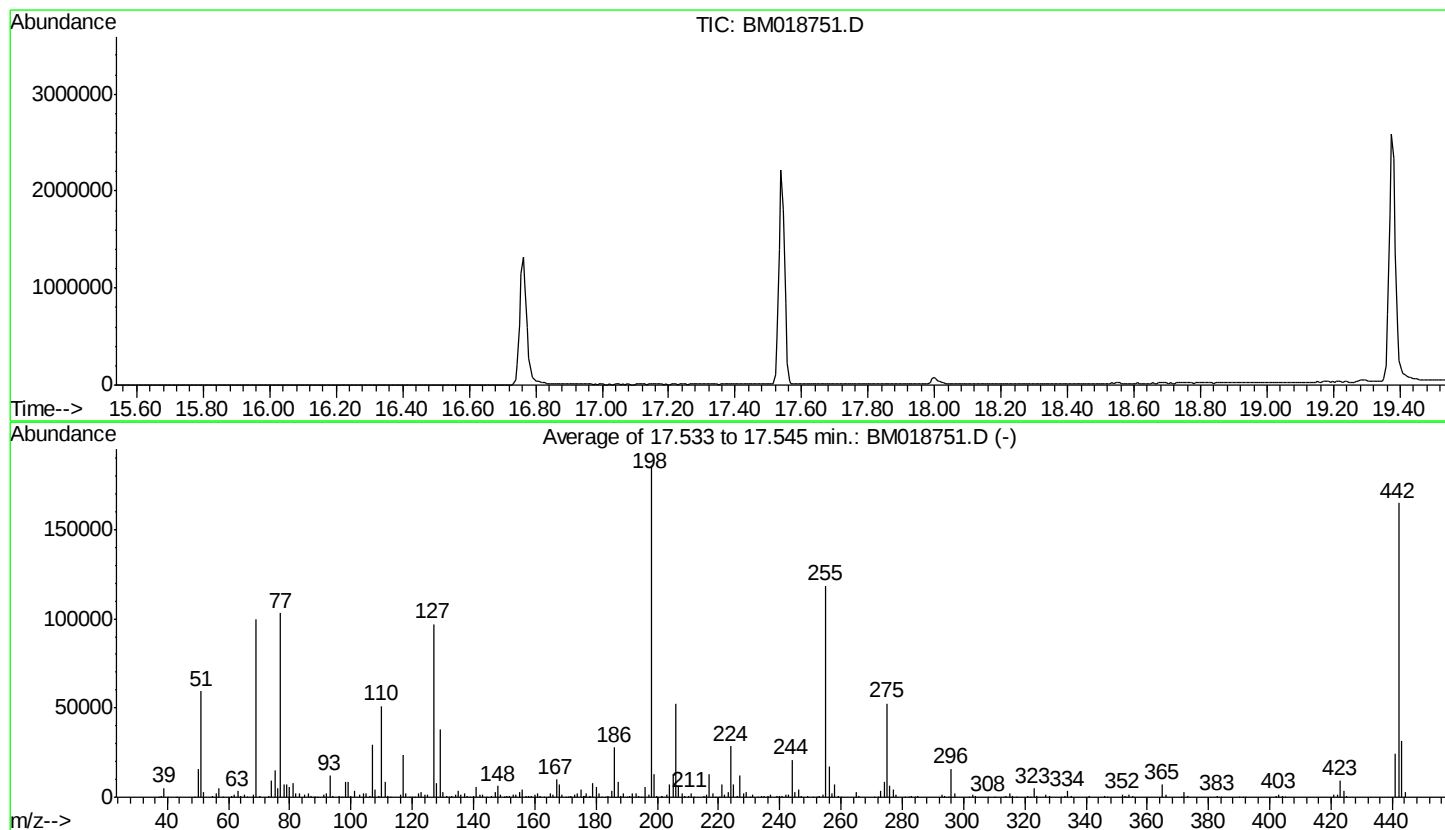

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	59461	PASS
68	69	0.00	2	1.7	1669	PASS
69	198	0.00	100	53.9	100074	PASS
70	69	0.00	2	0.5	542	PASS
127	198	10	80	52.2	97056	PASS
197	198	0.00	2	0.7	1340	PASS
198	198	100	100	100.0	185792	PASS
199	198	5	9	6.9	12855	PASS
275	198	10	60	28.2	52432	PASS
365	198	1	100	3.8	7089	PASS
441	198	0.01	100	13.3	24741	PASS
442	198	50	100	88.8	164917	PASS
443	442	15	24	19.3	31845	PASS