
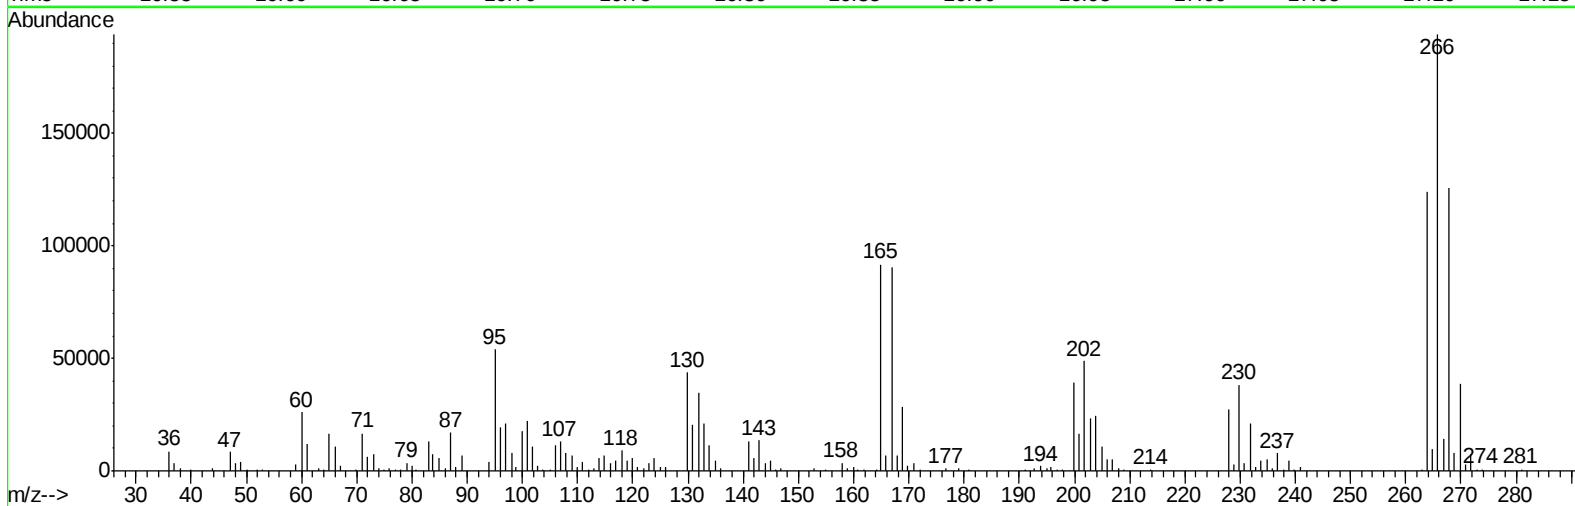


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021319\
Data File : BM018802.D
Acq On : 13 Feb 2019 14:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 07:04:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

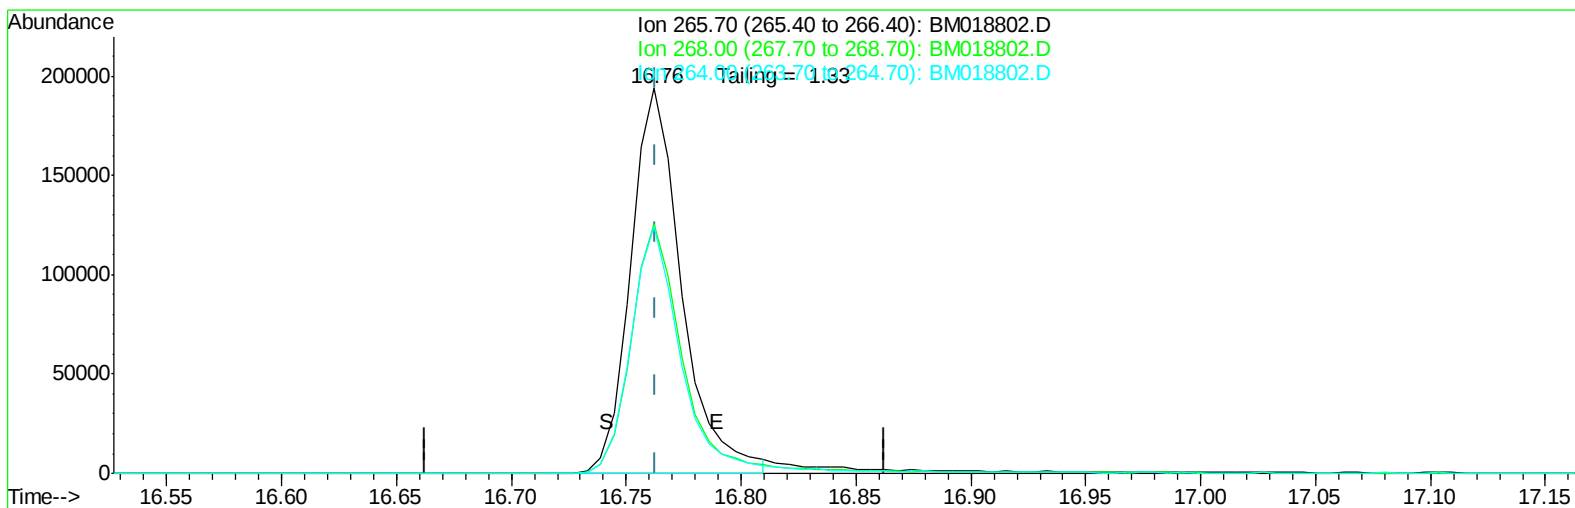

TIC: BM018802.D

(70) Pentachlorophenol (C)



16.762min (-0.000) 21824.25ng

response 303125

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	64.86
264.00	63.20	64.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021319\
Data File : BM018802.D
Acq On : 13 Feb 2019 14:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 07:04:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

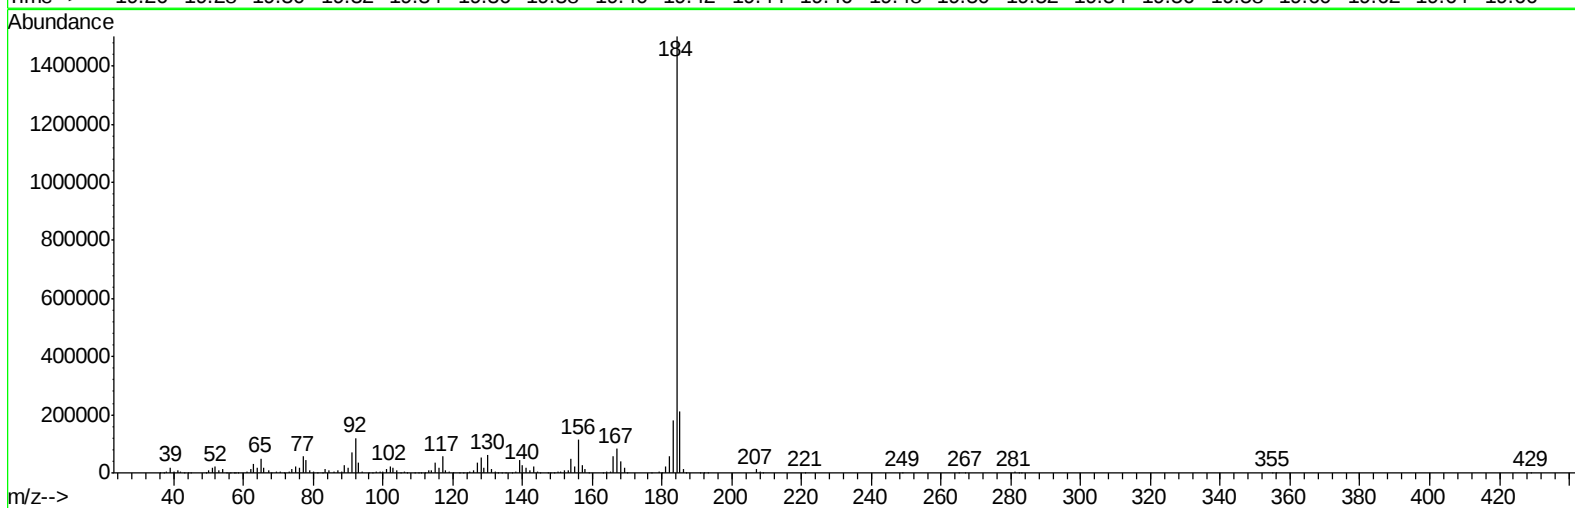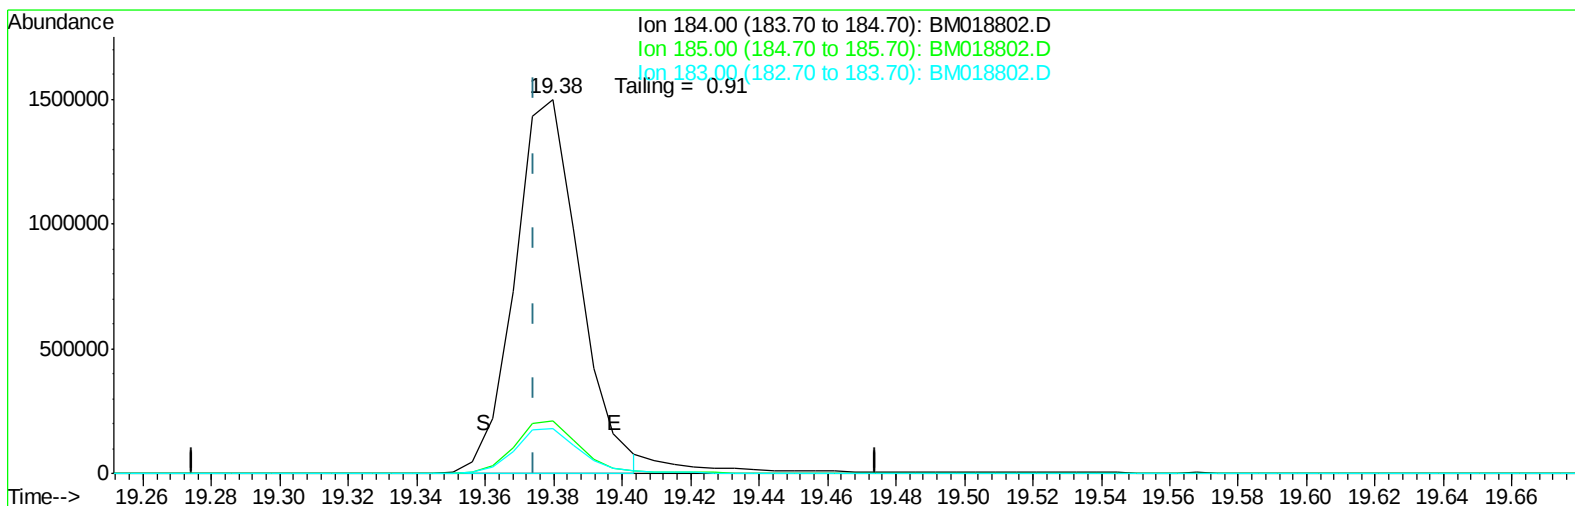

TIC: BM018802.D

(77) Benzidine

19.380min (+0.005) 29054.64ng

response 2038306

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.97
183.00	12.10	11.99
0.00	0.00	0.00