


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021319\
 Data File : BM018802.D
 Acq On : 13 Feb 2019 14:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 11 16:02:12 2019

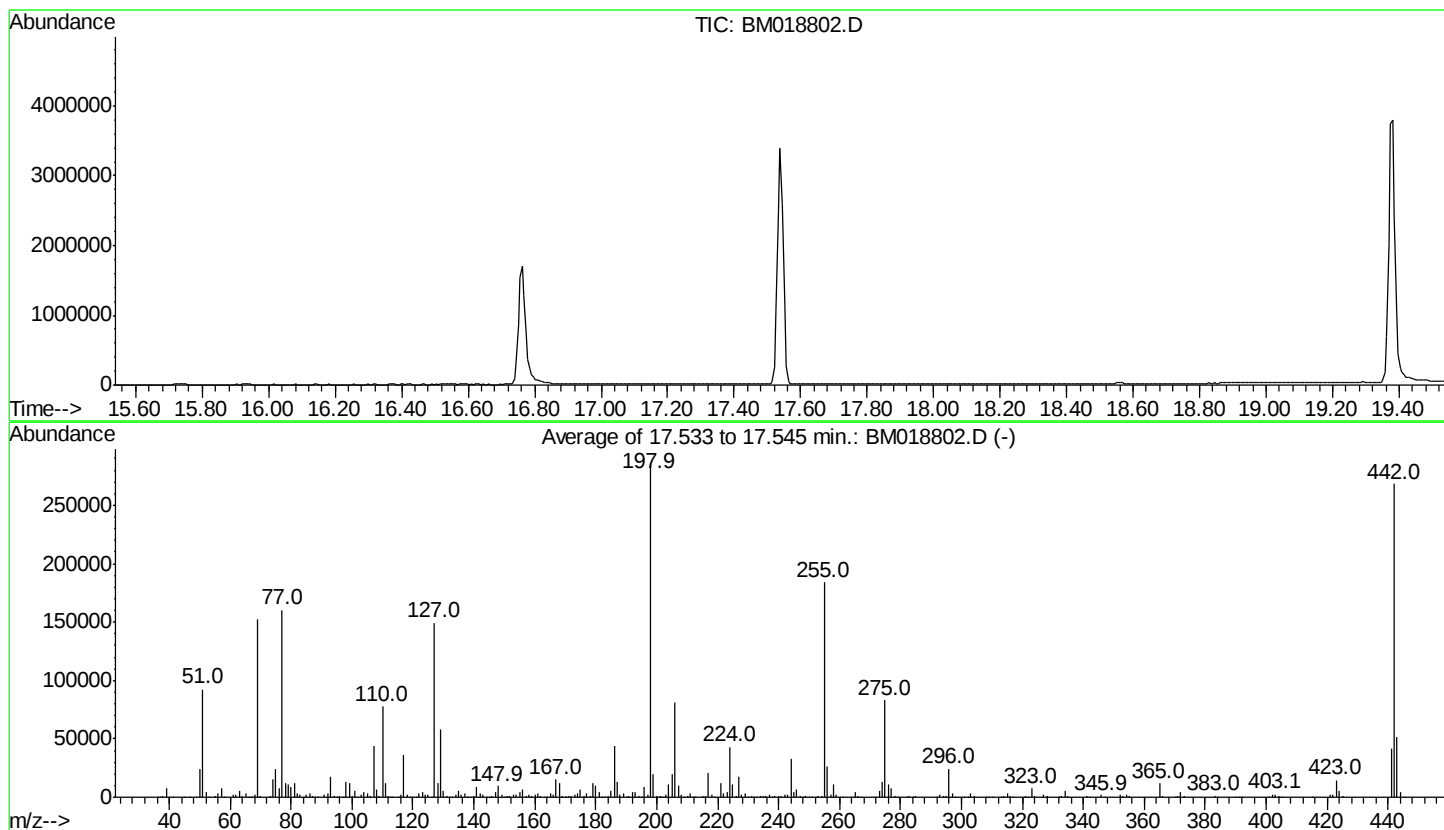

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	92440	PASS
68	69	0.00	2	1.8	2724	PASS
69	198	0.00	100	53.7	152626	PASS
70	69	0.00	2	0.5	803	PASS
127	198	10	80	52.7	149637	PASS
197	198	0.00	2	0.8	2134	PASS
198	198	100	100	100.0	283989	PASS
199	198	5	9	6.9	19608	PASS
275	198	10	60	29.2	82986	PASS
365	198	1	100	4.2	11874	PASS
441	198	0.01	100	14.6	41461	PASS
442	198	50	100	94.5	268330	PASS
443	442	15	24	19.3	51805	PASS