
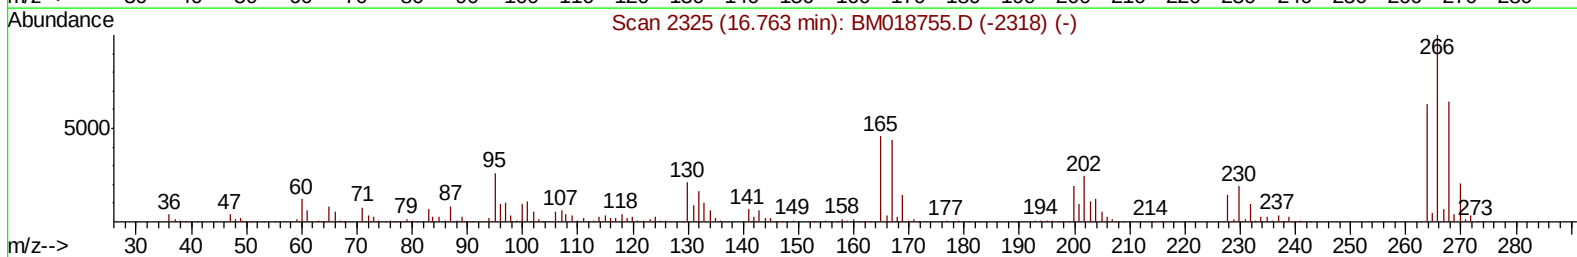
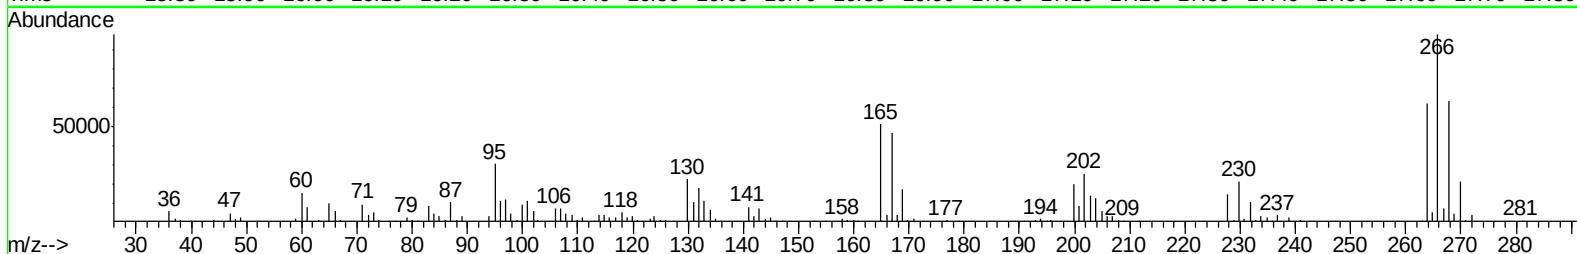


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021519\
Data File : BM018817.D
Acq On : 15 Feb 2019 14:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 03:38:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

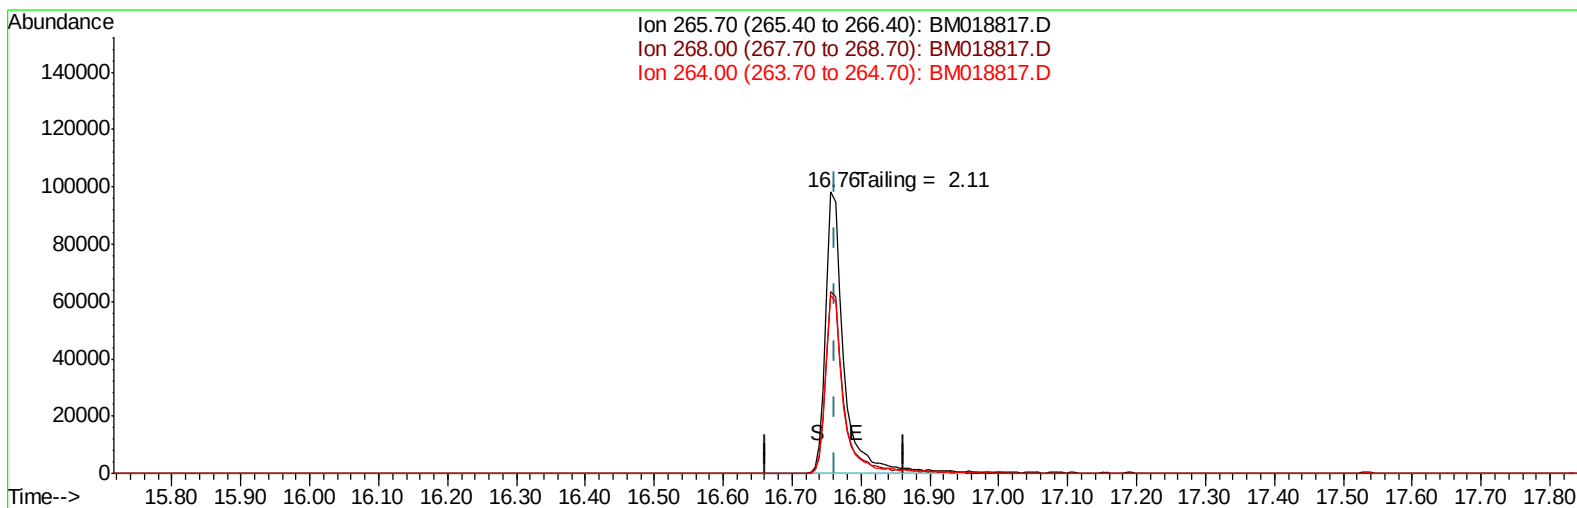

TIC: BM018817.D

(70) Pentachlorophenol (C)




16.757min (-0.006) 0.00ng

response 172673

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	64.45
264.00	63.20	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021519\
 Data File : BM018817.D
 Acq On : 15 Feb 2019 14:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 03:38:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 11 16:02:12 2019
 Response via : Initial Calibration

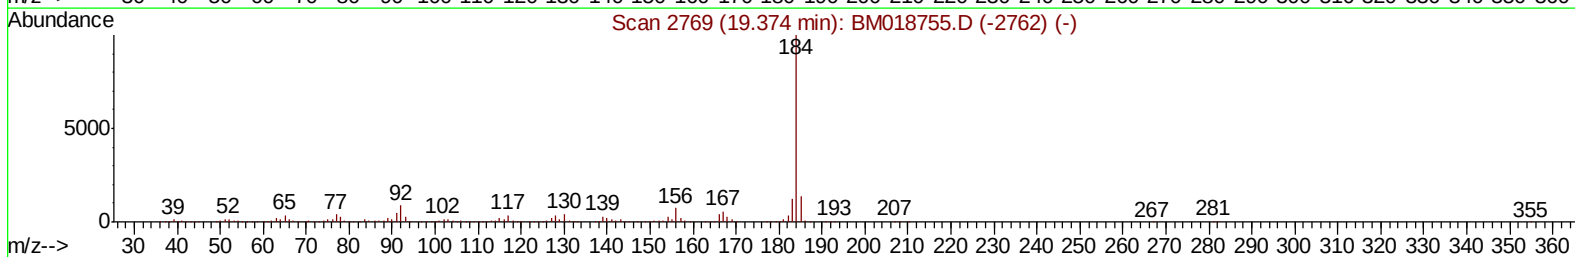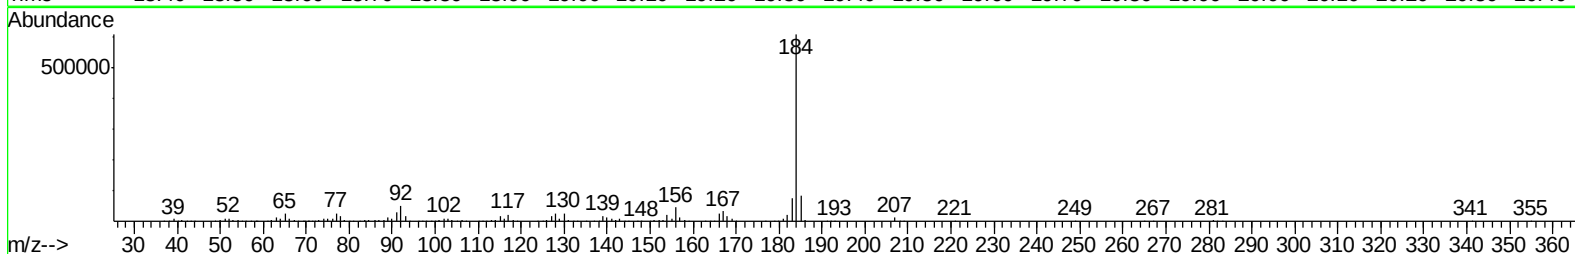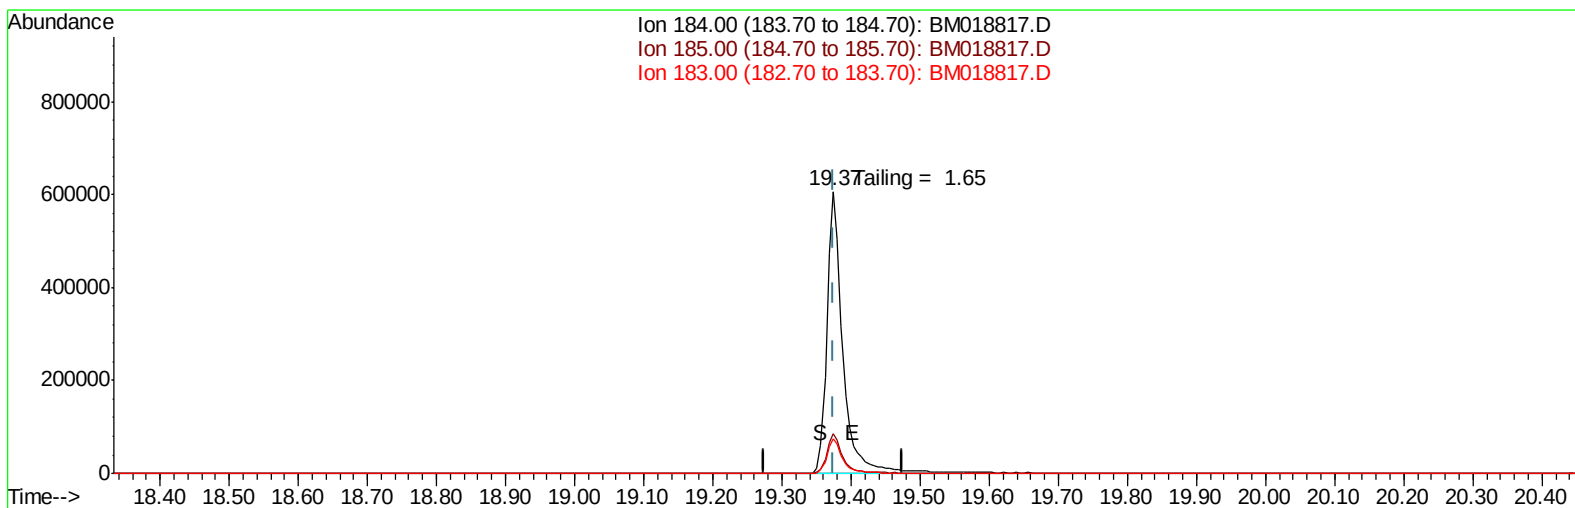

TIC: BM018817.D

(77) Benzidine

19.374min (-0.000) 0.00ng

response 946225

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.99
183.00	12.10	12.26
0.00	0.00	0.00