

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021519\
 Data File : BM018819.D
 Acq On : 15 Feb 2019 16:30
 Operator : JU/SJ
 Sample : K1500-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G-021419

Quant Time: Feb 15 23:03:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 11 16:02:12 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	277810	20.00	ng	-0.01
21) Naphthalene-d8	10.50	136	1112883	20.00	ng	0.00
39) Acenaphthene-d10	14.36	164	627757	20.00	ng	0.00
64) Phenanthrene-d10	17.11	188	1467260	20.00	ng	0.00
76) Chrysene-d12	21.30	240	1564517	20.00	ng	0.00
87) Perylene-d12	23.56	264	1541975	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	3167637	186.82	ng	0.00
7) Phenol-d6	6.89	99	4430079	185.47	ng	0.00
23) Nitrobenzene-d5	8.87	82	2824687	117.36	ng	-0.01
42) 2,4,6-Tribromophenol	15.86	330	1705170	188.44	ng	0.00
45) 2-Fluorobiphenyl	12.97	172	5541002	117.17	ng	0.00
79) Terphenyl-d14	19.74	244	8963387	118.19	ng	0.00
Target Compounds						
10) Phenol	6.91	94	79288	3.155	ng	77
50) Dimethylphthalate	13.82	163	293099	5.602	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021519\
Data File : BM018819.D
Acq On : 15 Feb 2019 16:30
Operator : JU/SJ
Sample : K1500-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G-021419

Quant Time: Feb 15 23:03:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

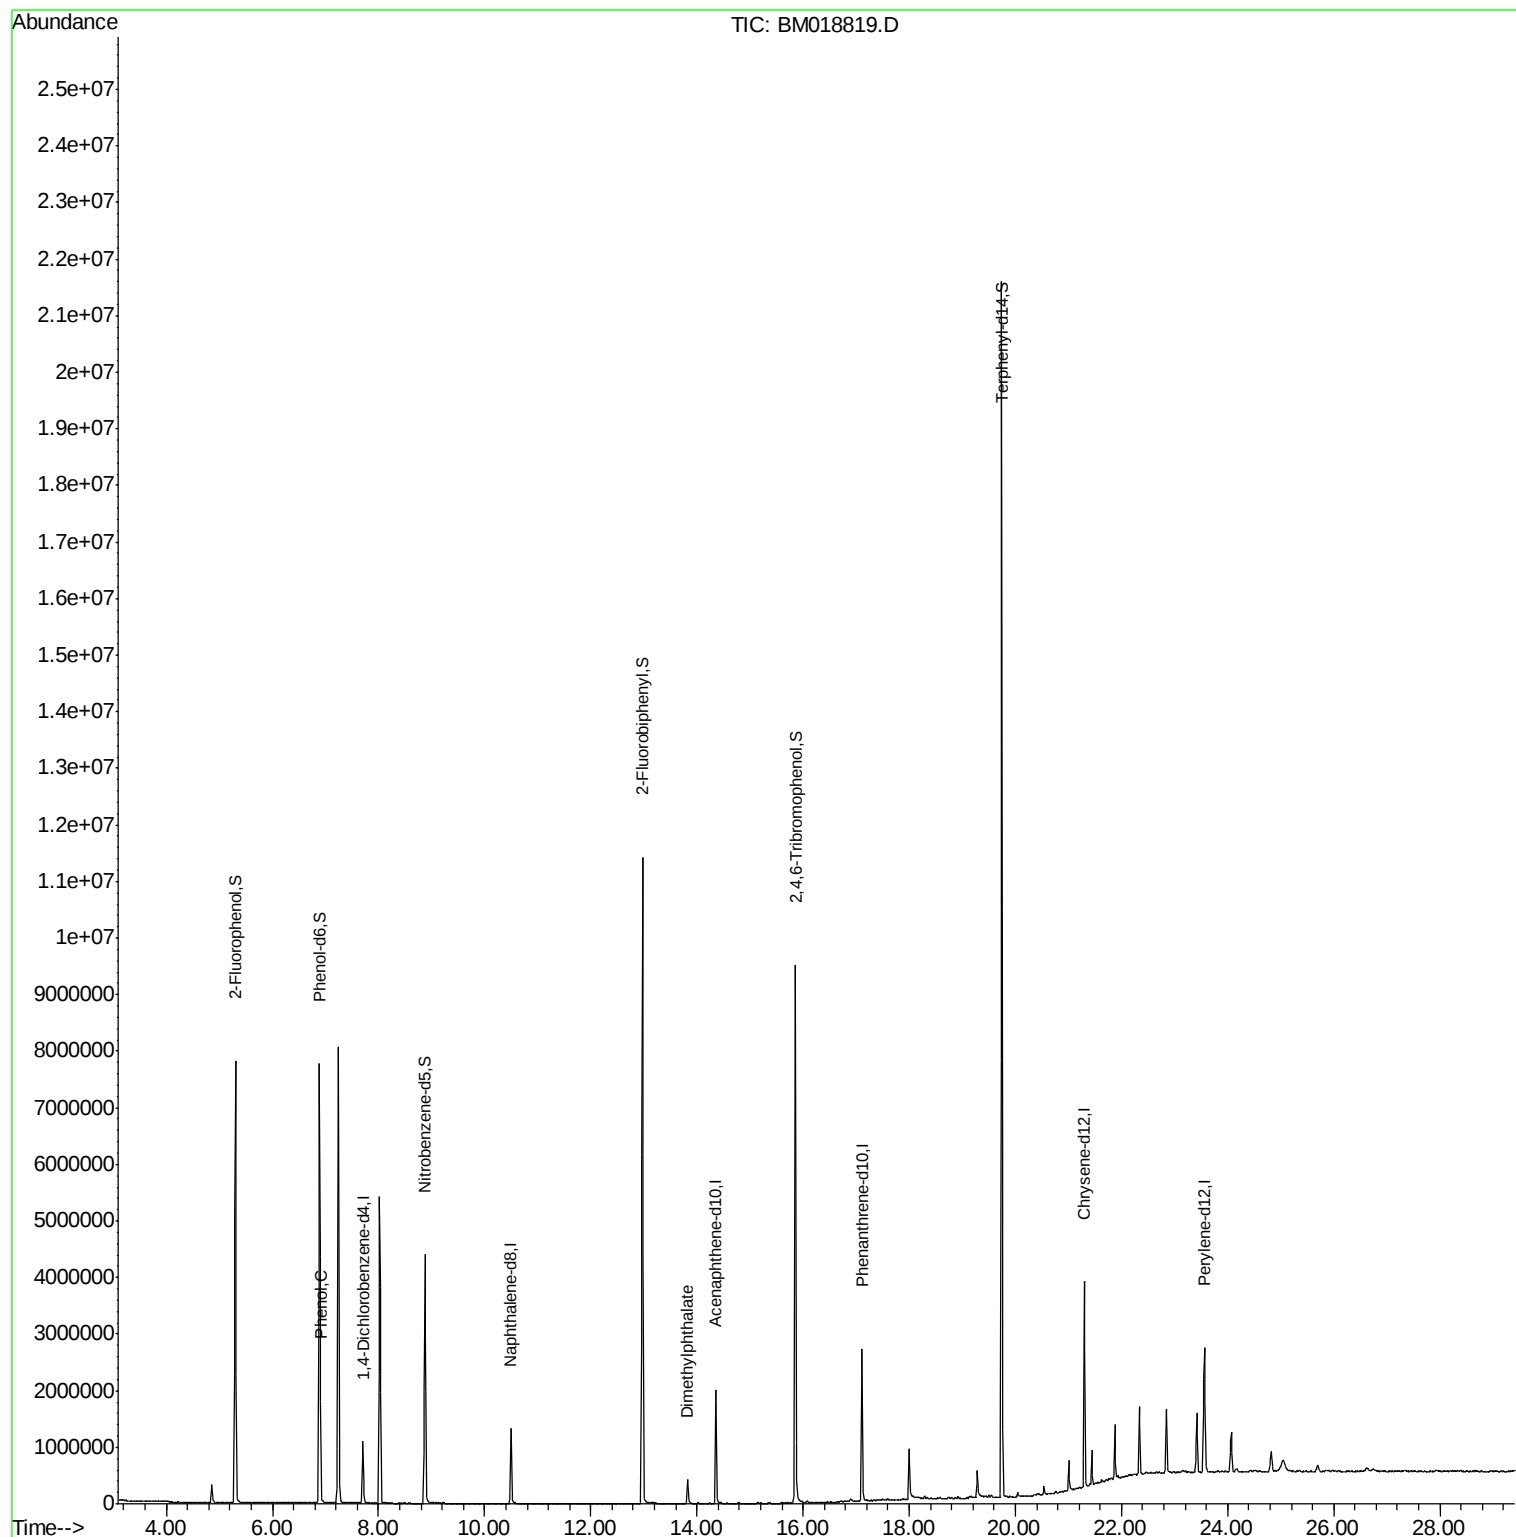




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.70 min Scan# 785
Delta R.T. -0.01 min
Lab File: BM018819.D
Acq: 15 Feb 2019 16:30

Instrument :
BNA_M
ClientSampleId :
G-021419

Tot Ion:152 Resp: 277810
Ion Ratio Lower Upper
152 100
150 157.0 127.3 190.9
115 65.5 50.8 76.2




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

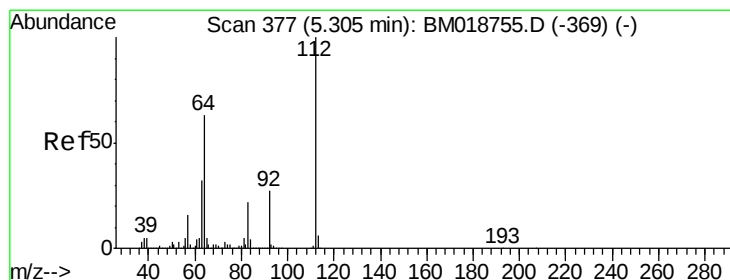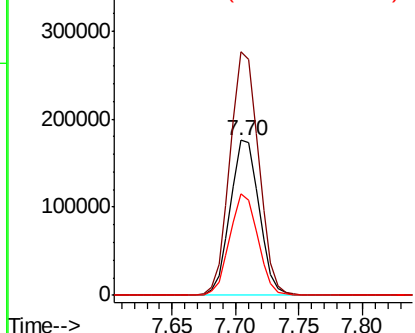



#5




2-Fluorophenol
Concen: 186.822 ng
RT: 5.30 min Scan# 377
Delta R.T. -0.00 min
Lab File: BM018819.D
Acq: 15 Feb 2019 16:30

Tgt Ion:112 Resp: 3167637
Ion Ratio Lower Upper
112 100
64 63.1 50.6 75.8
63 32.6 25.7 38.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

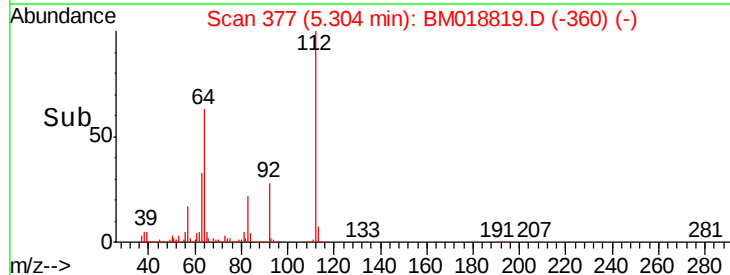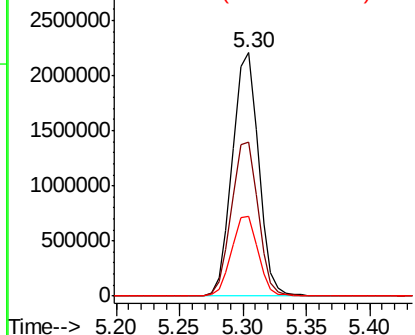

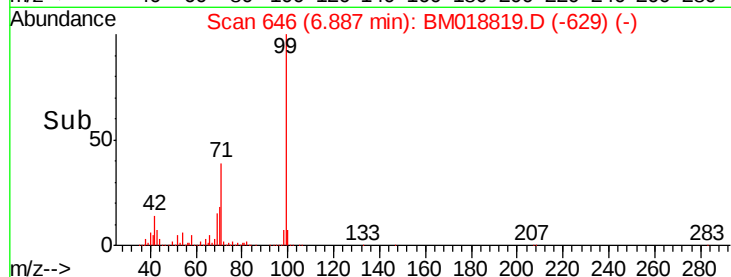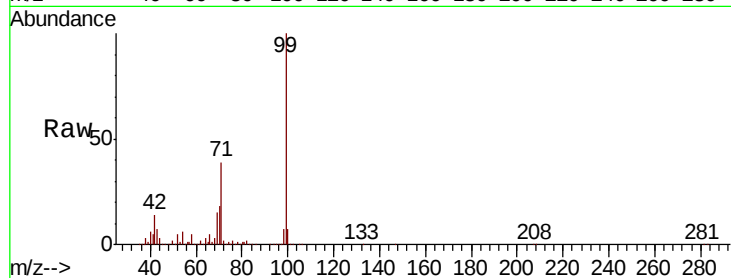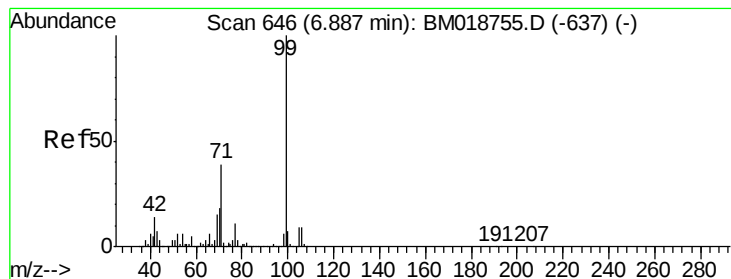

#7

Phenol-d6

Concen: 185.468 ng

RT: 6.89 min Scan# 646

Delta R.T. -0.00 min

Lab File: BM018819.D

Acq: 15 Feb 2019 16:30

Instrument :

BNA_M

ClientSampleId :

G-021419





Tot Ion: 99 Resp: 4430079

Ion Ratio Lower Upper

99 100

42 14.2 11.0 16.6

71 39.1 31.3 46.9

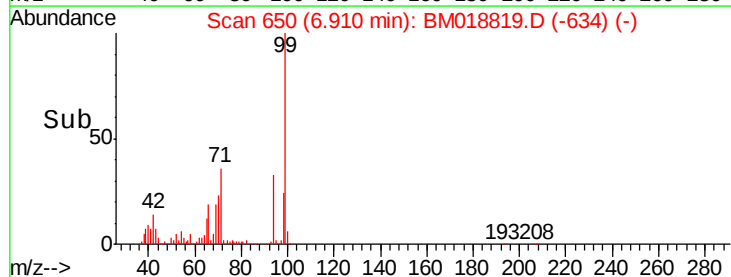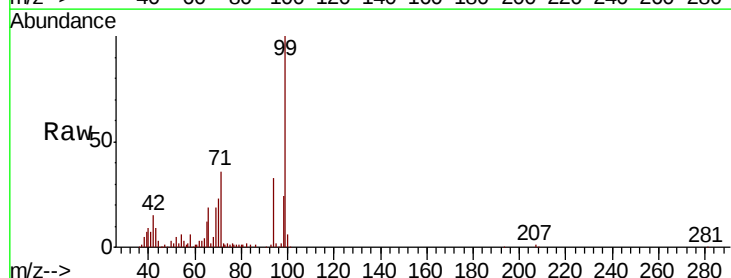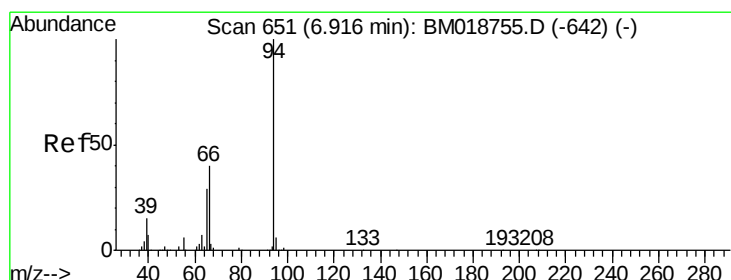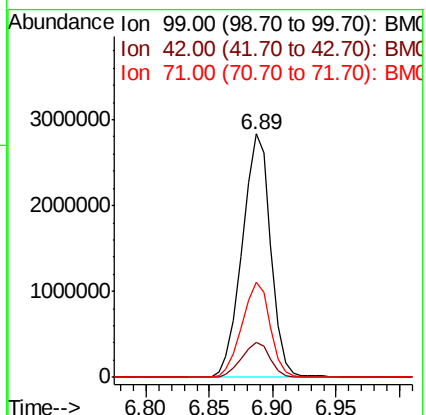

#10

Phenol

Concen: 3.155 ng

RT: 6.91 min Scan# 650

Delta R.T. -0.01 min

Lab File: BM018819.D

Acq: 15 Feb 2019 16:30


Tgt Ion: 94 Resp: 79288


Ion Ratio Lower Upper

94 100

65 37.0 9.6 49.6

66 59.1 20.4 60.4




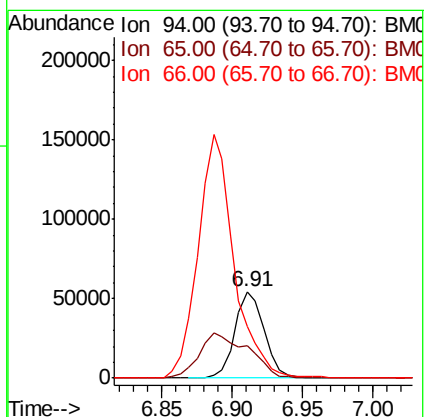




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.50 min Scan# 1260
Delta R.T. -0.01 min
Lab File: BM018819.D
Acq: 15 Feb 2019 16:30




Instrument :
BNA_M
ClientSampleId :
G-021419


Tot Ion:136	Resp: 1112883
Ion Ratio	Lower Upper
136 100	
137 10.5	8.8 13.2
54 6.3	5.0 7.6
68 7.0	5.5 8.3

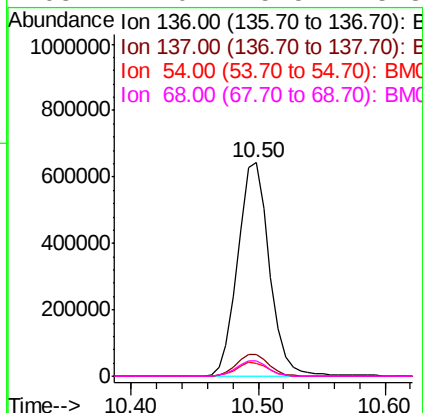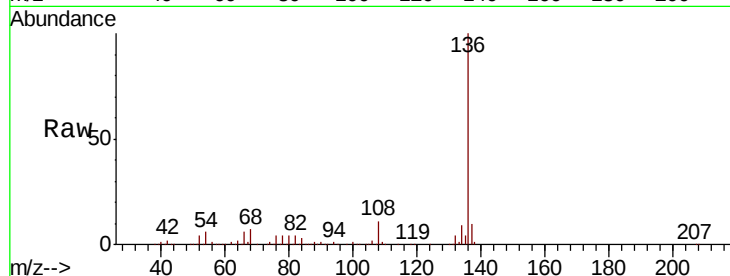

#23
Nitrobenzene-d5
Concen: 117.362 ng
RT: 8.87 min Scan# 984
Delta R.T. -0.01 min
Lab File: BM018819.D
Acq: 15 Feb 2019 16:30

Tgt Ion: 82	Resp: 2824687
Ion Ratio	Lower Upper
82 100	
128 36.2	29.9 44.9
54 37.1	29.1 43.7

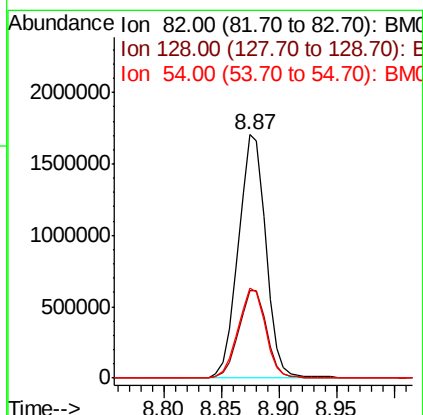



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.36 min Scan# 1916

Delta R.T. -0.01 min

Lab File: BM018819.D

Acq: 15 Feb 2019 16:30

Instrument :

BNA_M

ClientSampleId :

G-021419


Tot Ion:164 Resp: 627757

Ion Ratio Lower Upper

164 100

162 105.1 83.4 125.0




160 45.8 36.6 55.0



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

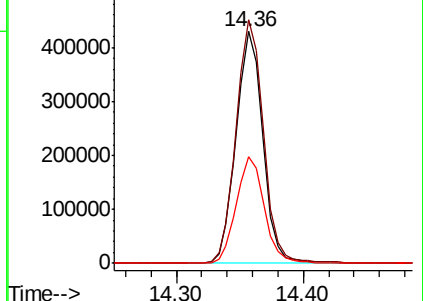

#42

2,4,6-Tribromophenol

Concen: 188.439 ng

RT: 15.86 min Scan# 2171

Delta R.T. -0.01 min

Lab File: BM018819.D

Acq: 15 Feb 2019 16:30


Tgt Ion:330 Resp: 1705170

Ion Ratio Lower Upper

330 100

332 96.4 76.9 115.3



141 35.8 28.7 43.1




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



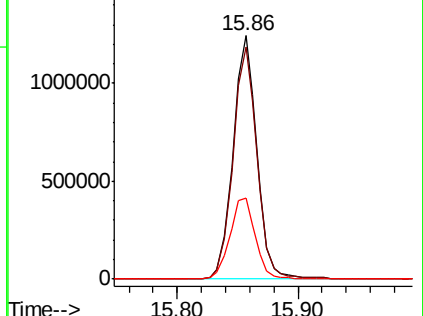





#45
2-Fluorobiphenyl
Concen: 117.172 ng
RT: 12.97 min Scan# 1681
Delta R.T. -0.01 min
Lab File: BM018819.D
Acq: 15 Feb 2019 16:30




Instrument :
BNA_M
ClientSampleId :
G-021419

Tot Ion:172 Resp: 5541002
Ion Ratio Lower Upper
172 100
171 36.0 29.0 43.6
170 23.5 18.6 28.0

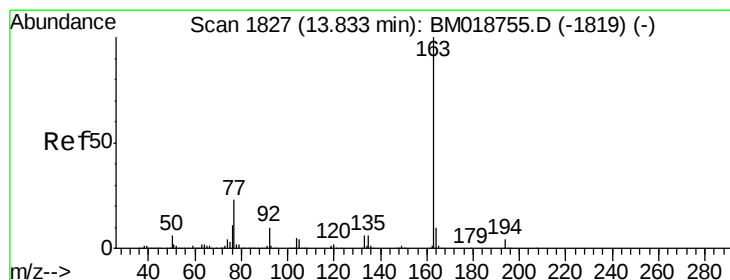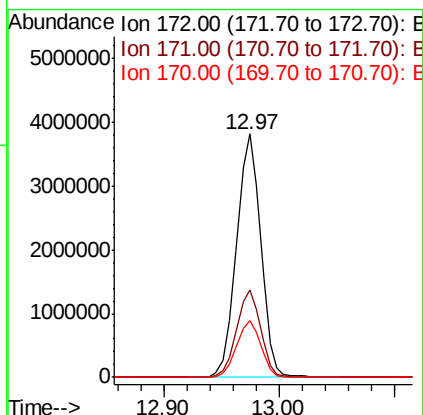

#50
Dimethylphthalate
Concen: 5.602 ng
RT: 13.82 min Scan# 1825
Delta R.T. -0.01 min
Lab File: BM018819.D
Acq: 15 Feb 2019 16:30

Tgt Ion:163 Resp: 293099
Ion Ratio Lower Upper
163 100
194 3.8 3.2 4.8
164 9.5 7.8 11.8

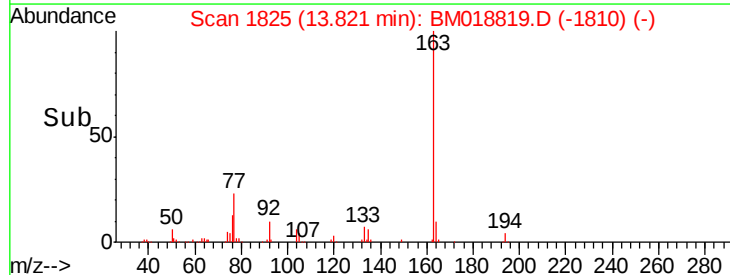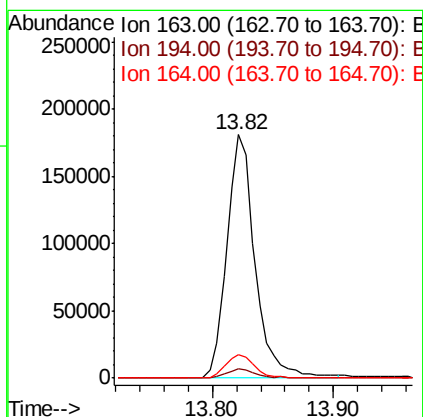



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.11 min Scan# 2384

Delta R.T. -0.01 min

Lab File: BM018819.D

Acq: 15 Feb 2019 16:30

Instrument :

BNA_M

ClientSampleId :

G-021419


Tot Ion:188 Resp: 1467260

Ion Ratio Lower Upper

188 100

94 10.4 8.2 12.2




80 12.2 9.7 14.5

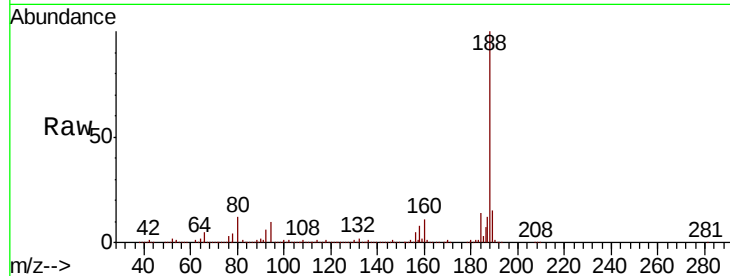

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

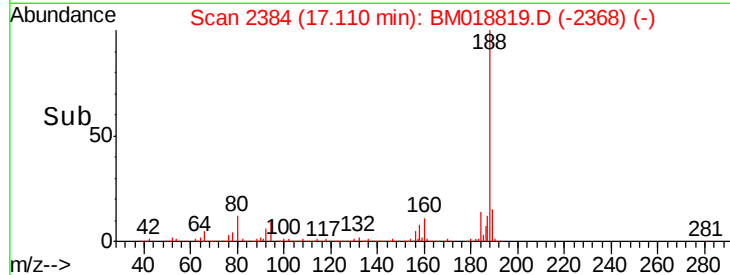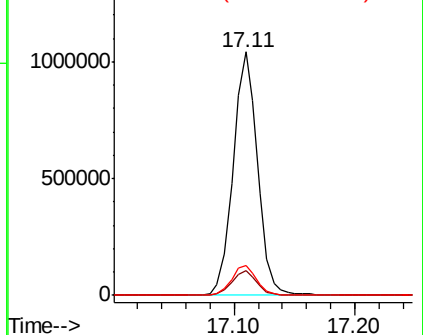

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.30 min Scan# 3097

Delta R.T. -0.01 min

Lab File: BM018819.D

Acq: 15 Feb 2019 16:30


Tgt Ion:240 Resp: 1564517

Ion Ratio Lower Upper

240 100

120 11.4 8.9 13.3



236 25.6 20.9 31.3

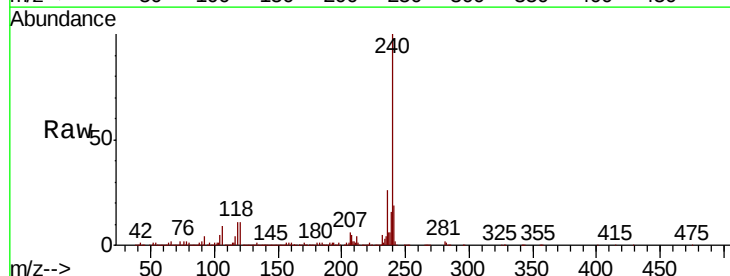


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

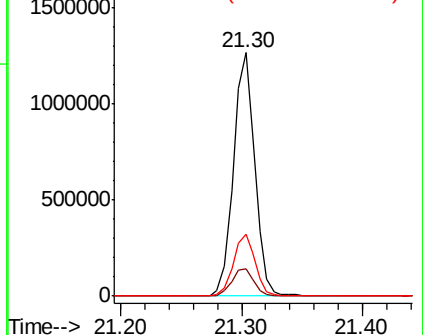


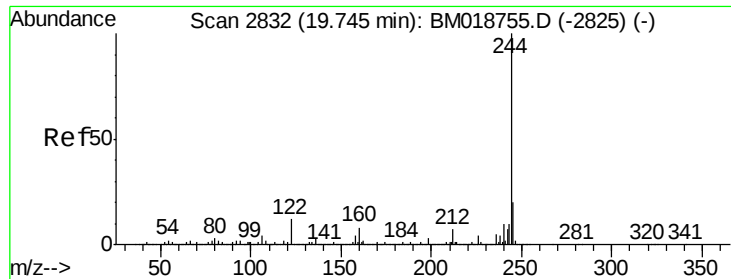




#79
 Terphenyl-d14
 Concen: 118.187 ng
 RT: 19.74 min Scan# 2832
 Delta R.T. -0.00 min
 Lab File: BM018819.D
 Acq: 15 Feb 2019 16:30

Instrument :
 BNA_M
 ClientSampleId :
 G-021419

Tot Ion:244 Resp: 8963387
 Ion Ratio Lower Upper
 244 100
 212 7.3 5.6 8.4
 122 11.9 9.3 13.9

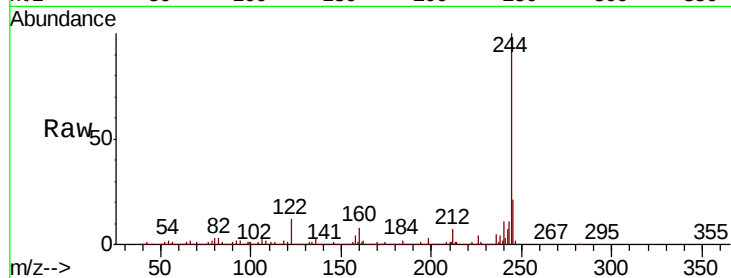


Abundance Ion 244.00 (243.70 to 244.70): E
 1e+07 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

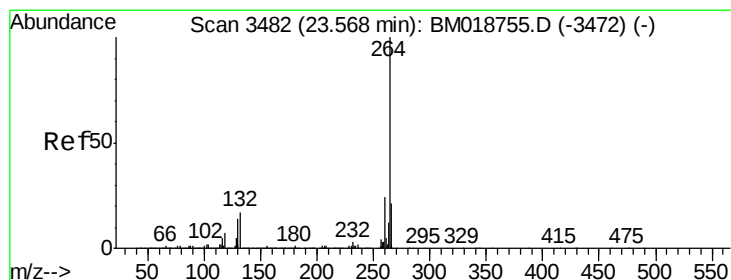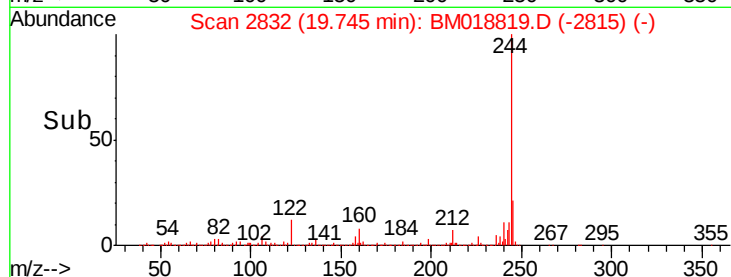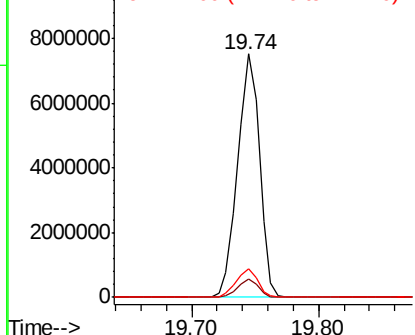

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.56 min Scan# 3481
 Delta R.T. -0.01 min
 Lab File: BM018819.D
 Acq: 15 Feb 2019 16:30

Tgt Ion:264 Resp: 1541975
 Ion Ratio Lower Upper
 264 100
 260 23.8 18.9 28.3
 265 21.5 17.3 25.9

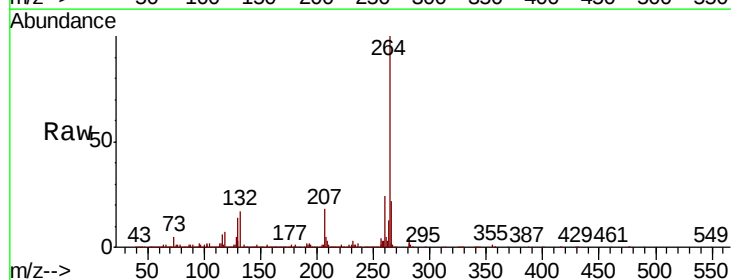

Abundance Ion 264.00 (263.70 to 264.70): E
 1000000 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

