


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021519\
 Data File : BM018817.D
 Acq On : 15 Feb 2019 14:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 11 16:02:12 2019

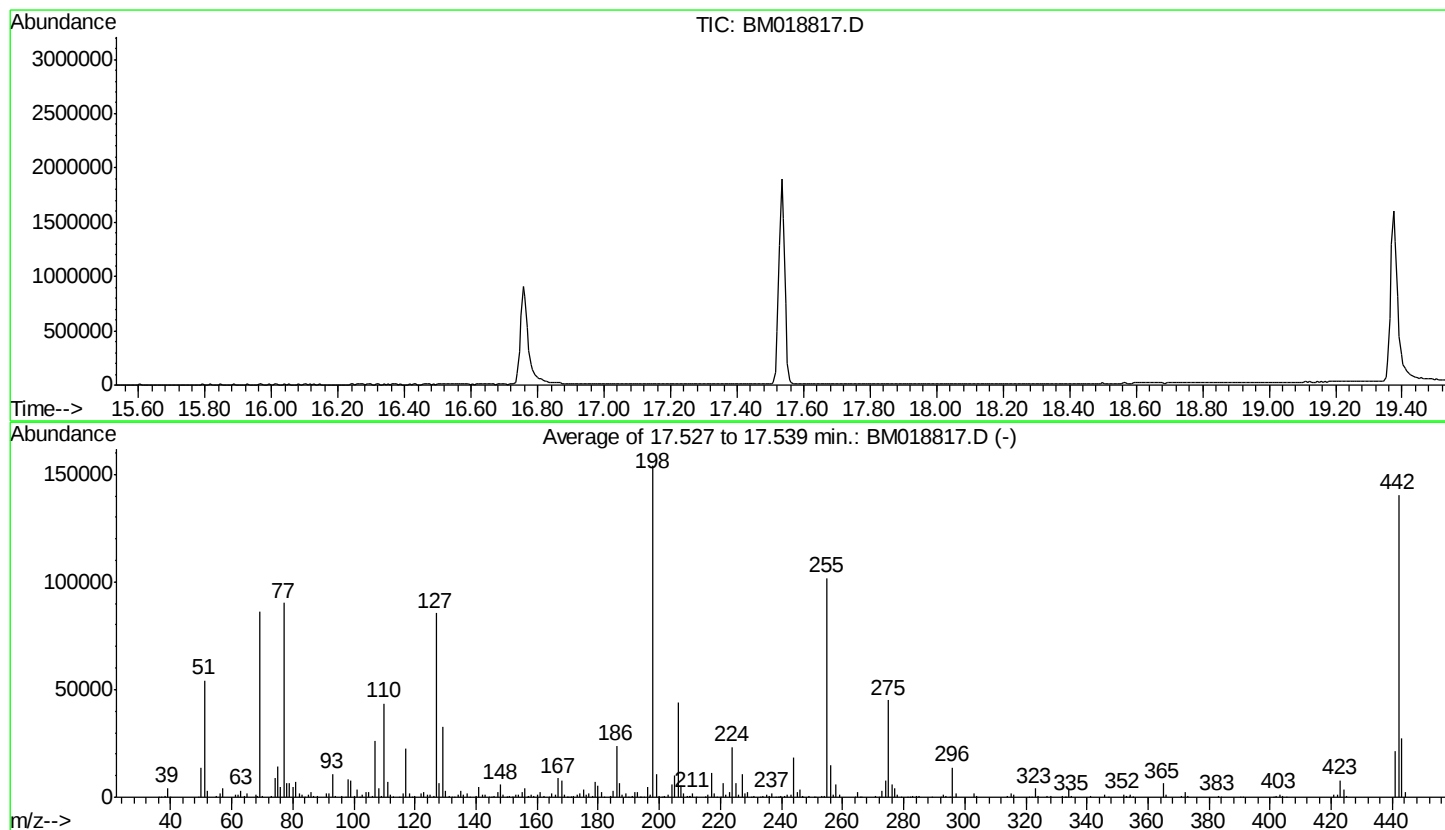

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	54162	PASS
68	69	0.00	2	1.5	1270	PASS
69	198	0.00	100	56.0	86189	PASS
70	69	0.00	2	0.4	335	PASS
127	198	10	80	55.4	85376	PASS
197	198	0.00	2	0.7	1032	PASS
198	198	100	100	100.0	154016	PASS
199	198	5	9	7.1	10982	PASS
275	198	10	60	29.3	45144	PASS
365	198	1	100	4.2	6416	PASS
441	198	0.01	100	13.9	21413	PASS
442	198	50	100	91.1	140346	PASS
443	442	15	24	19.6	27554	PASS