
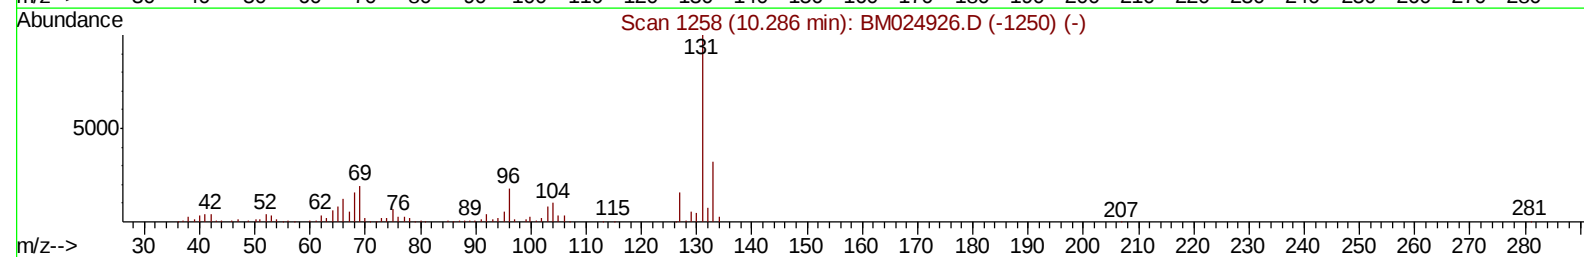
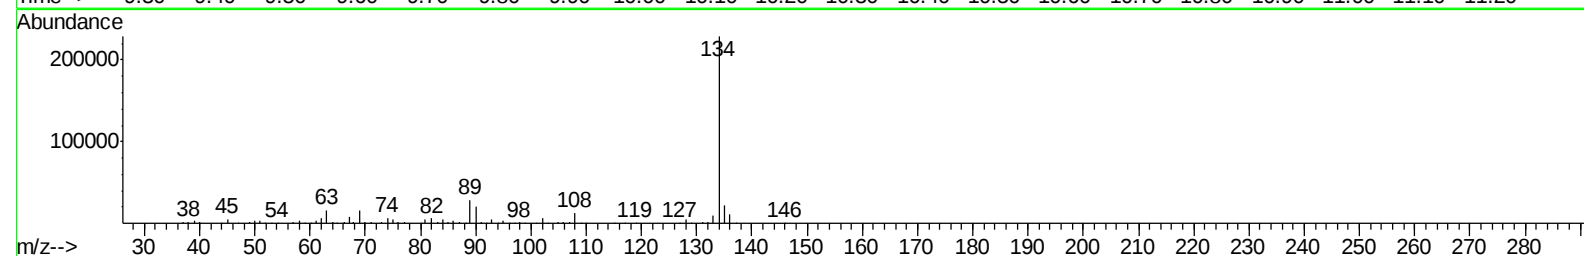


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021720\
Data File : BM024929.D
Acq On : 18 Feb 2020 14:22
Operator : CG/JU
Sample : L1486-07DL 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Feb 19 03:42:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 03:36:08 2020
Response via : Initial Calibration

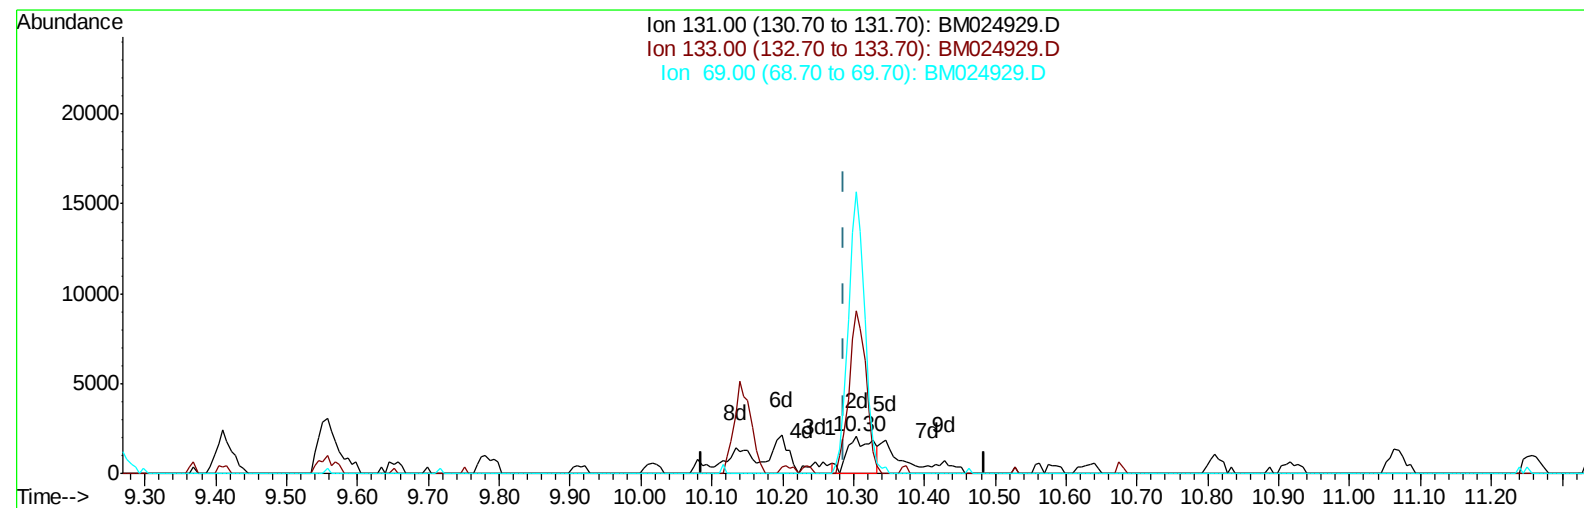

TIC: BM024929.D

(29) 4-Chloroaniline-d4 (S)

10.304min (+0.018) 0.28ng/ul m

response 5179

Ion	Exp%	Act%
131.00	100	100
133.00	34.60	443.66#
69.00	16.20	767.21#
0.00	0.00	0.00