

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021720\
 Data File : BM024931.D
 Acq On : 18 Feb 2020 15:34
 Operator : CG/JU
 Sample : L1486-06DL2 100X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBCT6DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.646	128	129	132	rBV3	3722	3885	0.11%	0.016%
2	3.716	135	141	145	rBV4	11757	25608	0.69%	0.106%
3	4.881	334	339	341	rBV5	3044	4732	0.13%	0.020%
4	6.510	612	616	619	rBV4	3243	5195	0.14%	0.022%
5	6.757	652	658	662	rBV5	5899	12154	0.33%	0.050%
6	6.939	686	689	693	rBV4	4588	6304	0.17%	0.026%
7	7.057	704	709	714	rBV3	8301	14811	0.40%	0.061%
8	7.387	759	765	776	rBV	1059191	1772314	47.93%	7.348%
9	7.510	784	786	790	rVB3	4298	4301	0.12%	0.018%
10	7.757	823	828	837	rBV	43101	69880	1.89%	0.290%
11	7.916	847	855	862	rBV	61360	101887	2.76%	0.422%
12	8.557	958	964	970	rBV6	7660	14528	0.39%	0.060%
13	8.733	990	994	998	rVB5	4726	7275	0.20%	0.030%
14	8.863	1008	1016	1020	rBV6	9183	22000	0.59%	0.091%
15	9.557	1129	1134	1138	rBV4	7377	11981	0.32%	0.050%
16	9.651	1148	1150	1153	rBV4	3717	3832	0.10%	0.016%
17	10.139	1226	1233	1237	rBV	1367888	2303160	62.28%	9.548%
18	10.186	1237	1241	1256	rVV	2133628	3667406	99.17%	15.204%
19	10.304	1256	1261	1268	rVV	59027	101552	2.75%	0.421%
20	11.116	1396	1399	1403	rBV4	2360	4085	0.11%	0.017%
21	11.710	1495	1500	1505	rBV2	5687	9254	0.25%	0.038%
22	11.822	1513	1519	1529	rBV	132552	260651	7.05%	1.081%
23	12.045	1548	1557	1563	rBV	98154	171721	4.64%	0.712%
24	12.869	1692	1697	1704	rBV2	32560	56749	1.53%	0.235%
25	13.069	1726	1731	1735	rBV4	7420	12491	0.34%	0.052%
26	13.204	1748	1754	1762	rVB7	6562	17328	0.47%	0.072%
27	13.357	1775	1780	1785	rBV3	15354	24830	0.67%	0.103%
28	13.416	1785	1790	1794	rVB5	3720	6268	0.17%	0.026%
29	13.468	1794	1799	1805	rBV	12237	23757	0.64%	0.098%
30	13.598	1818	1821	1823	rBV3	5374	5692	0.15%	0.024%
31	13.616	1823	1824	1831	rVB4	4093	5429	0.15%	0.023%
32	13.727	1837	1843	1846	rBV	21342	34145	0.92%	0.142%
33	13.763	1846	1849	1854	rVB5	4550	6192	0.17%	0.026%
34	14.039	1889	1896	1902	rBV	1950307	2990214	80.86%	12.397%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021720\
 Data File : BM024931.D
 Acq On : 18 Feb 2020 15:34
 Operator : CG/JU
 Sample : L1486-06DL2 100X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBCT6DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Title : SVOA CALIBRATION

35	14.098	1902	1906	1915	rVV	313341	475764	12.87%	1.972%
36	14.180	1915	1920	1931	rVB	39500	76336	2.06%	0.316%
37	14.357	1946	1950	1956	rVB3	6066	9398	0.25%	0.039%
38	14.445	1960	1965	1978	rVV	147941	283932	7.68%	1.177%
39	14.539	1978	1981	1987	rVB6	3386	5566	0.15%	0.023%
40	14.892	2037	2041	2044	rBV4	2735	4456	0.12%	0.018%
41	15.045	2062	2067	2072	rBV2	26737	39463	1.07%	0.164%
42	15.098	2072	2076	2083	rVB	63010	88797	2.40%	0.368%
43	15.268	2102	2105	2110	rVB6	7432	10878	0.29%	0.045%
44	15.357	2116	2120	2125	rVV6	4545	7495	0.20%	0.031%
45	15.404	2125	2128	2135	rVB3	11566	15553	0.42%	0.064%
46	15.551	2149	2153	2155	rBV2	10270	11796	0.32%	0.049%
47	15.774	2185	2191	2201	rBV3	33565	57786	1.56%	0.240%
48	15.898	2210	2212	2218	rVB6	4208	5293	0.14%	0.022%
49	16.580	2324	2328	2330	rBV2	7438	9026	0.24%	0.037%
50	16.609	2330	2333	2340	rVB2	15321	22442	0.61%	0.093%
51	16.792	2358	2364	2369	rBV	2317918	3331720	90.09%	13.812%
52	16.833	2369	2371	2378	rVV	218972	289237	7.82%	1.199%
53	16.898	2378	2382	2394	rVB3	34612	74392	2.01%	0.308%
54	17.209	2430	2435	2447	rBV2	40424	82930	2.24%	0.344%
55	17.686	2512	2516	2517	rBV3	3739	4157	0.11%	0.017%
56	17.727	2520	2523	2529	rBV6	8869	17190	0.46%	0.071%
57	17.868	2542	2547	2551	rBV2	10904	18417	0.50%	0.076%
58	18.339	2624	2627	2630	rVV5	2619	3974	0.11%	0.016%
59	18.874	2712	2718	2724	rBV2	21506	46577	1.26%	0.193%
60	19.203	2769	2774	2783	rBV2	37774	84363	2.28%	0.350%
61	21.009	3075	3081	3091	rBV	2689938	3698047	100.00%	15.331%
62	23.103	3431	3437	3447	rVB	2024573	3564491	96.39%	14.777%




Sum of corrected areas: 24121087

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021720\
Data File : BM024931.D
Acq On : 18 Feb 2020 15:34
Operator : CG/JU
Sample : L1486-06DL2 100X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBCT6DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

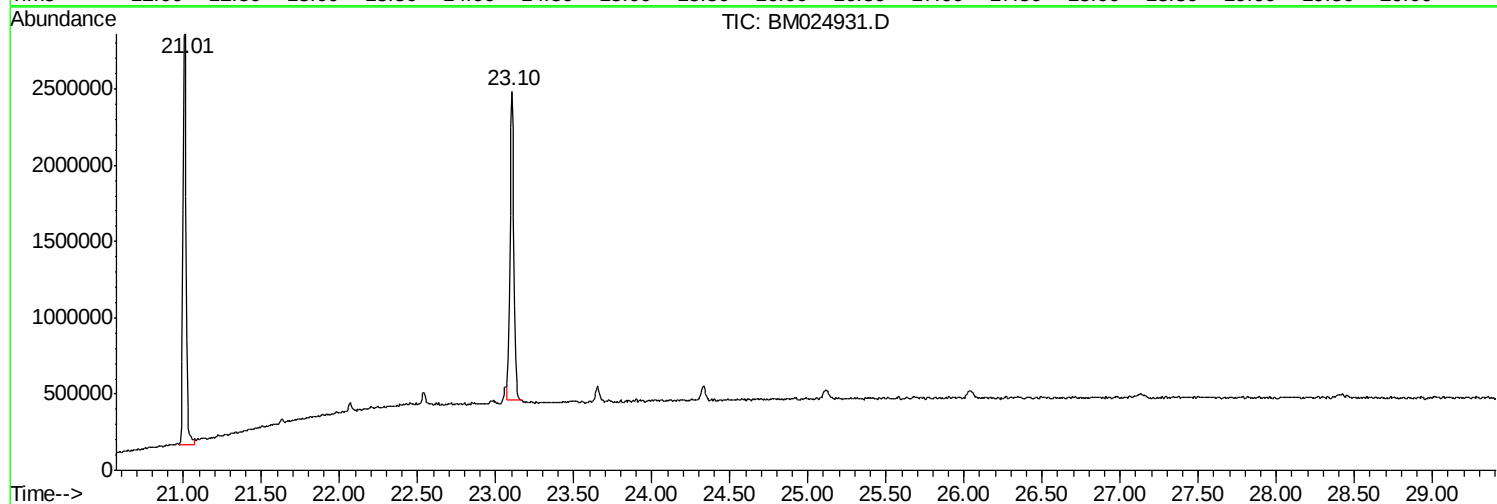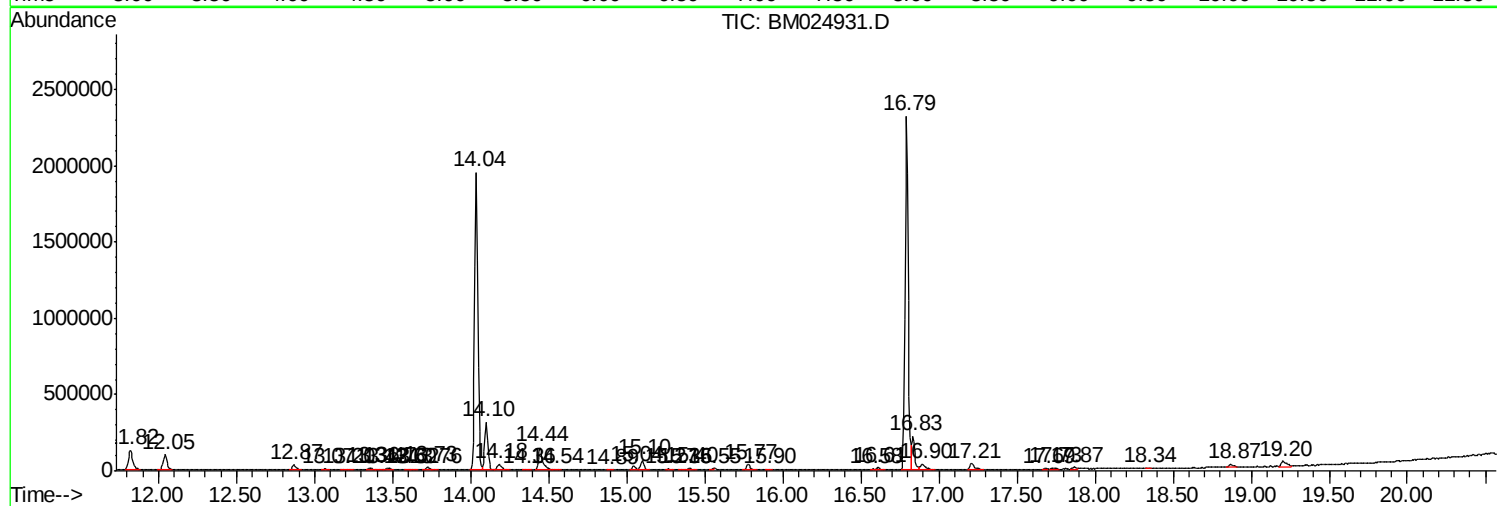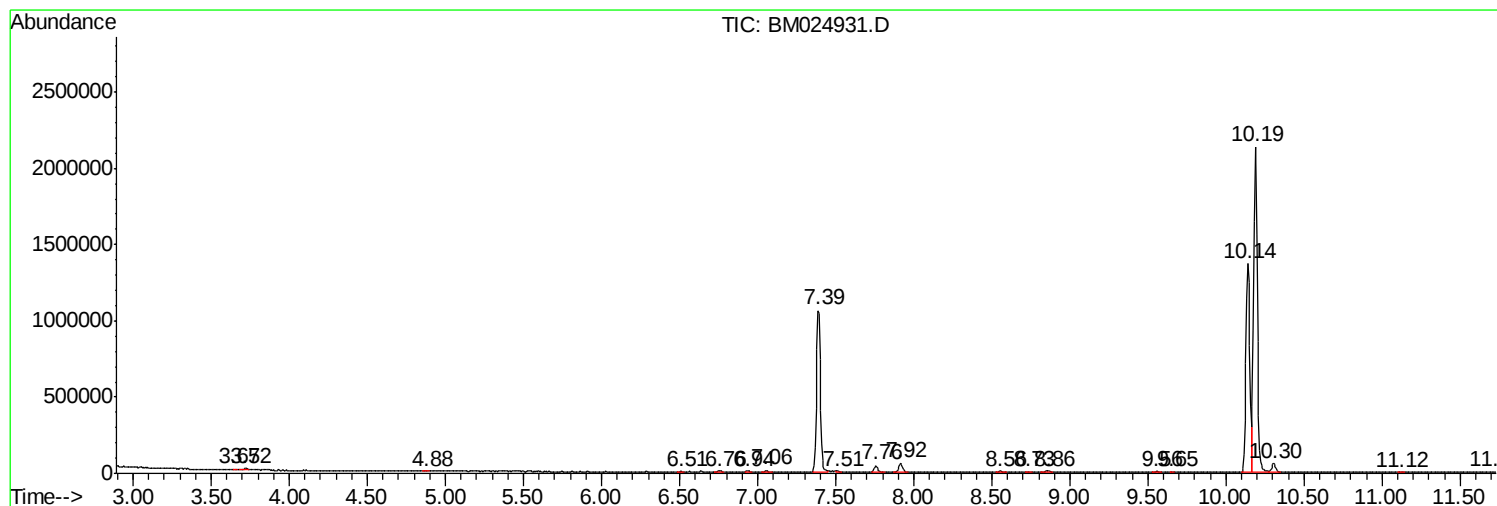

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM021720\
Data File : BM024931.D
Acq On : 18 Feb 2020 15:34
Operator : CG/JU
Sample : L1486-06DL2 100X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBCT6DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM021720\
Data File : BM024931.D
Acq On : 18 Feb 2020 15:34
Operator : CG/JU
Sample : L1486-06DL2 100X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBCT6DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc