

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021720\
 Data File : BM024932.D
 Acq On : 18 Feb 2020 16:10
 Operator : CG/JU
 Sample : L1486-07DL2 100X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBCT7DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.716	137	141	148	rVB5	9873	22526	0.60%	0.099%
2	5.457	434	437	442	rBV6	2634	4891	0.13%	0.021%
3	6.640	636	638	644	rBV5	2443	3907	0.10%	0.017%
4	6.757	654	658	662	rBV3	5179	7965	0.21%	0.035%
5	6.939	685	689	694	rBV4	5412	9226	0.24%	0.040%
6	7.057	706	709	714	rVB4	7519	9514	0.25%	0.042%
7	7.175	727	729	734	rBV4	2089	3914	0.10%	0.017%
8	7.387	758	765	778	rBV	1102420	1824487	48.42%	8.003%
9	7.504	782	785	791	rVV6	3897	7454	0.20%	0.033%
10	7.757	823	828	837	rVB2	34011	53866	1.43%	0.236%
11	7.916	846	855	863	rBV	41773	74744	1.98%	0.328%
12	8.557	958	964	965	rBV3	6191	7465	0.20%	0.033%
13	8.728	990	993	994	rBV3	4360	4391	0.12%	0.019%
14	8.857	1010	1015	1021	rBV6	6155	13865	0.37%	0.061%
15	8.928	1021	1027	1029	rVB4	2333	4248	0.11%	0.019%
16	10.139	1226	1233	1237	rBV	1383832	2295618	60.93%	10.070%
17	10.186	1237	1241	1257	rVV	1552531	2662159	70.66%	11.678%
18	10.310	1257	1262	1269	rVB2	40466	71924	1.91%	0.315%
19	11.716	1495	1501	1504	rBV5	3430	5971	0.16%	0.026%
20	11.822	1513	1519	1527	rBV	88369	174668	4.64%	0.766%
21	12.045	1547	1557	1567	rBV	69342	128381	3.41%	0.563%
22	12.869	1692	1697	1707	rVB	26883	47264	1.25%	0.207%
23	13.069	1727	1731	1733	rBV2	6502	8172	0.22%	0.036%
24	13.204	1747	1754	1758	rBV6	5104	10410	0.28%	0.046%
25	13.363	1775	1781	1786	rBV2	13813	22209	0.59%	0.097%
26	13.474	1794	1800	1806	rBV	13279	23313	0.62%	0.102%
27	13.604	1817	1822	1824	rBV3	3839	5772	0.15%	0.025%
28	13.727	1835	1843	1846	rBV	18498	27307	0.72%	0.120%
29	13.757	1846	1848	1853	rVB4	2875	3819	0.10%	0.017%
30	14.039	1889	1896	1902	rBV	2021820	2998495	79.58%	13.153%
31	14.098	1902	1906	1913	rVV	266618	398853	10.59%	1.750%
32	14.186	1916	1921	1930	rVB	29852	54785	1.45%	0.240%
33	14.357	1943	1950	1954	rBV3	5836	9519	0.25%	0.042%
34	14.445	1959	1965	1983	rBV	116285	232906	6.18%	1.022%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021720\
 Data File : BM024932.D
 Acq On : 18 Feb 2020 16:10
 Operator : CG/JU
 Sample : L1486-07DL2 100X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBCT7DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Title : SVOA CALIBRATION

35	15.045	2061	2067	2071	rBV	26294	36977	0.98%	0.162%
36	15.104	2071	2077	2084	rVB3	44512	72715	1.93%	0.319%
37	15.221	2095	2097	2101	rVB4	3567	4652	0.12%	0.020%
38	15.268	2101	2105	2109	rVB4	6322	9938	0.26%	0.044%
39	15.351	2116	2119	2124	rVB3	3507	4283	0.11%	0.019%
40	15.404	2124	2128	2134	rBV2	8769	12152	0.32%	0.053%
41	15.557	2148	2154	2157	rBV3	9188	14399	0.38%	0.063%
42	15.780	2187	2192	2202	rVB4	24187	40275	1.07%	0.177%
43	16.580	2324	2328	2331	rBV	5407	10245	0.27%	0.045%
44	16.609	2331	2333	2338	rVB	12620	16290	0.43%	0.071%
45	16.792	2358	2364	2369	rBV	2379224	3344498	88.76%	14.671%
46	16.833	2369	2371	2378	rVV	184658	245839	6.52%	1.078%
47	16.892	2378	2381	2390	rVB2	32361	58199	1.54%	0.255%
48	17.209	2430	2435	2442	rBV	27472	55148	1.46%	0.242%
49	17.674	2510	2514	2519	rBV5	4178	8237	0.22%	0.036%
50	17.727	2520	2523	2525	rBV4	4101	4281	0.11%	0.019%
51	17.862	2542	2546	2553	rBV5	10510	20088	0.53%	0.088%
52	18.868	2713	2717	2722	rBV2	16655	23134	0.61%	0.101%
53	19.203	2770	2774	2778	rBV2	28376	46841	1.24%	0.205%
54	19.427	2811	2812	2814	rBV2	6823	6052	0.16%	0.027%
55	21.009	3075	3081	3093	rBV	2840864	3767827	100.00%	16.528%
56	23.103	3431	3437	3447	rVB	2166224	3761198	99.82%	16.498%


Sum of corrected areas: 22797276

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021720\
Data File : BM024932.D
Acq On : 18 Feb 2020 16:10
Operator : CG/JU
Sample : L1486-07DL2 100X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBCT7DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

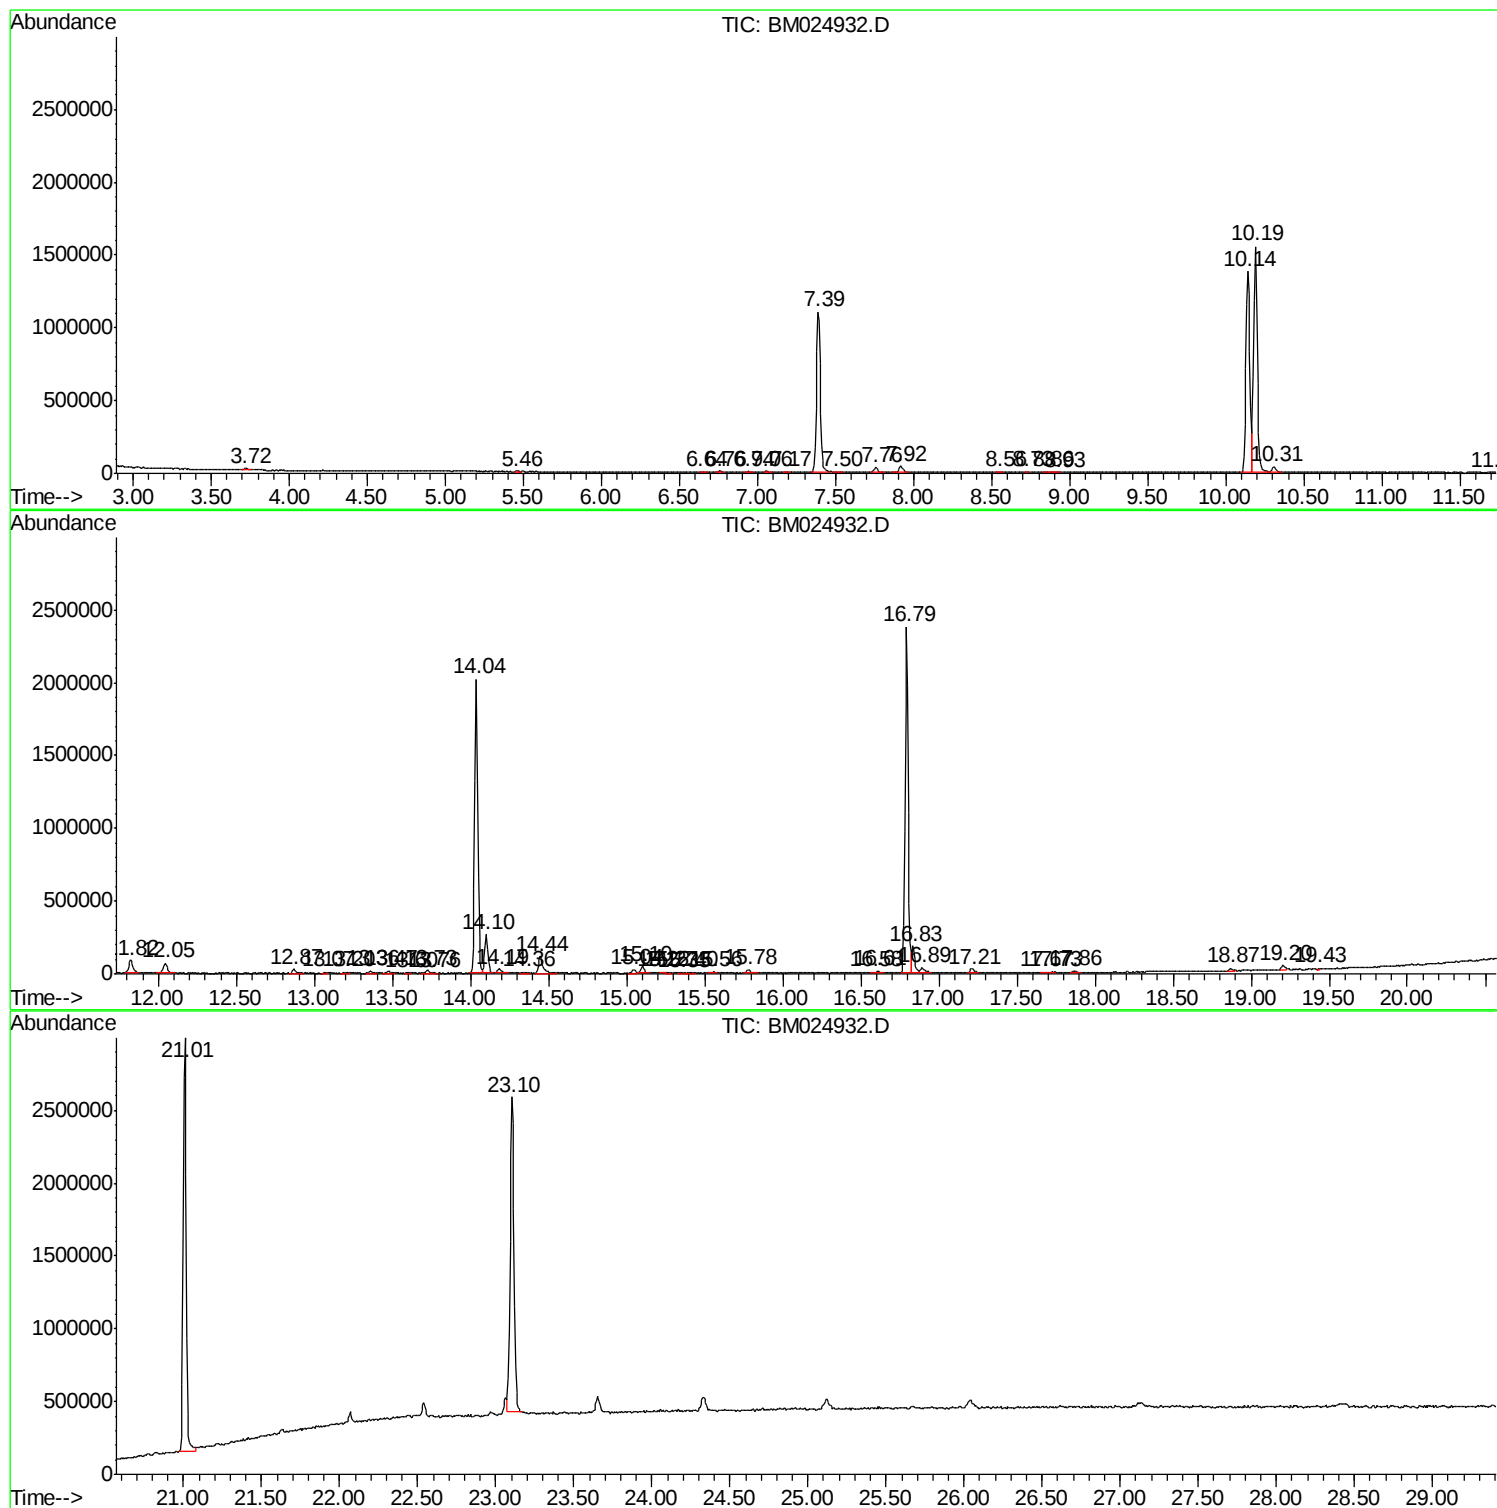

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM021720\
Data File : BM024932.D
Acq On : 18 Feb 2020 16:10
Operator : CG/JU
Sample : L1486-07DL2 100X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBCT7DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM021720\
Data File : BM024932.D
Acq On : 18 Feb 2020 16:10
Operator : CG/JU
Sample : L1486-07DL2 100X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBCT7DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc