
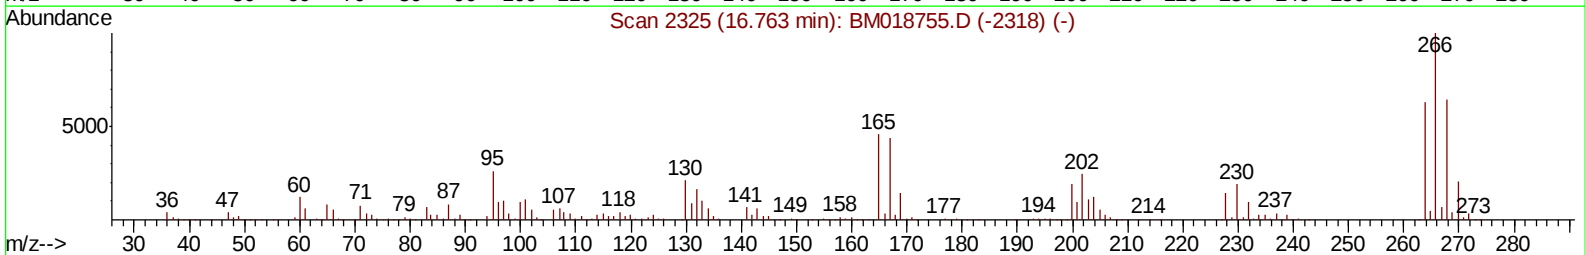
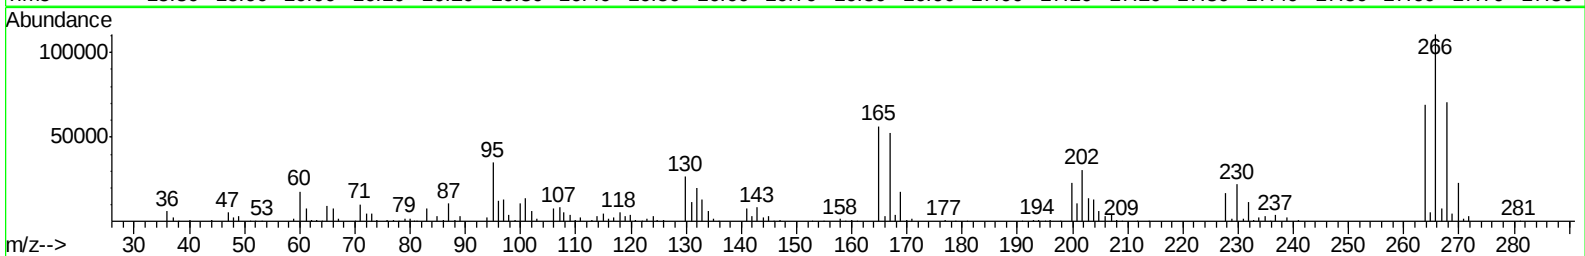


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM021919\
Data File : BM018868.D
Acq On : 19 Feb 2019 23:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 06:04:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

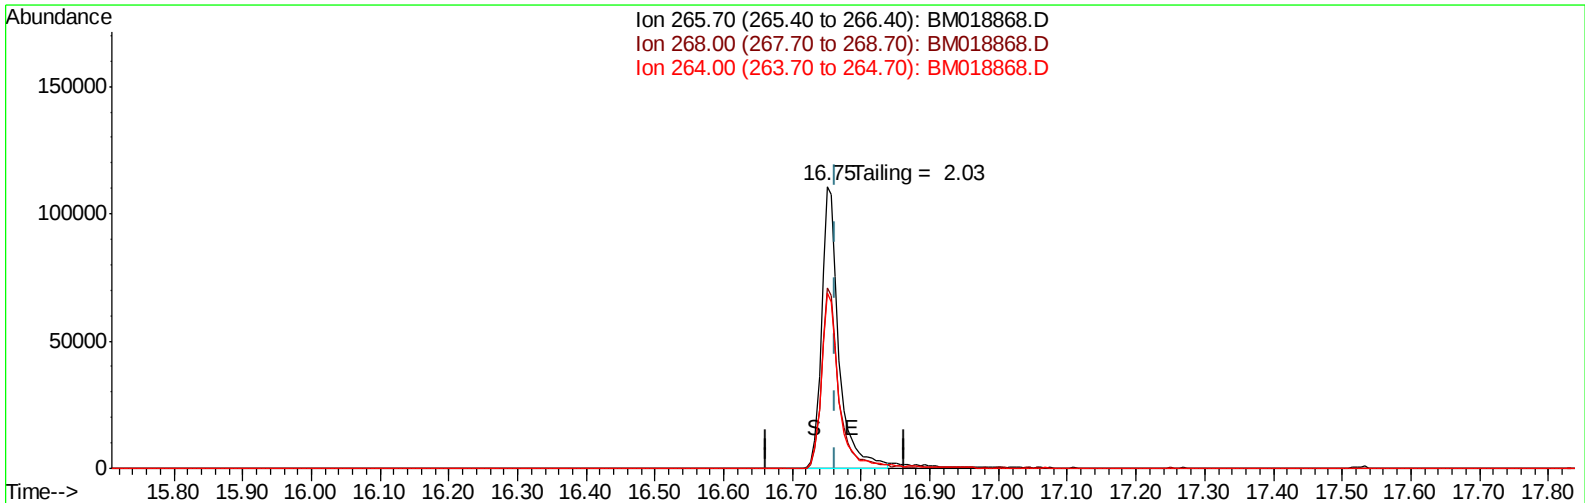

TIC: BM018868.D

(70) Pentachlorophenol (C)




16.751min (-0.012) 92880.90ng

response 194520

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	64.01
264.00	63.20	62.17
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM021919\
 Data File : BM018868.D
 Acq On : 19 Feb 2019 23:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 06:04:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 11 16:02:12 2019
 Response via : Initial Calibration

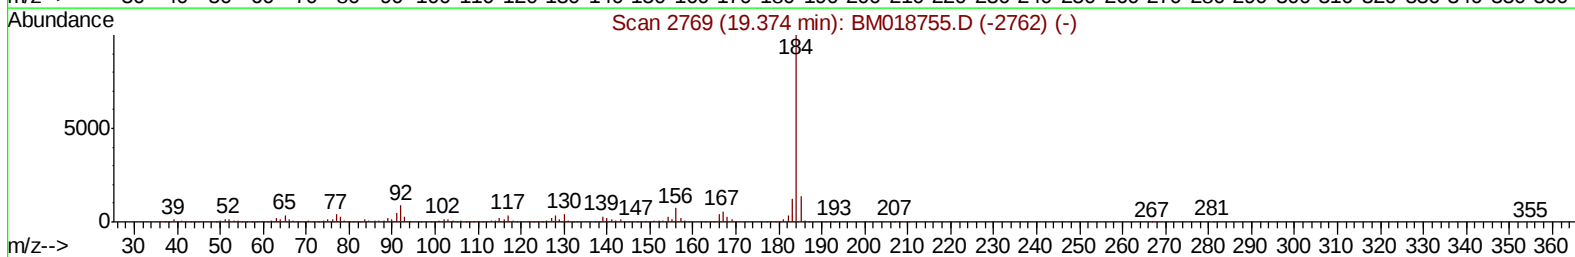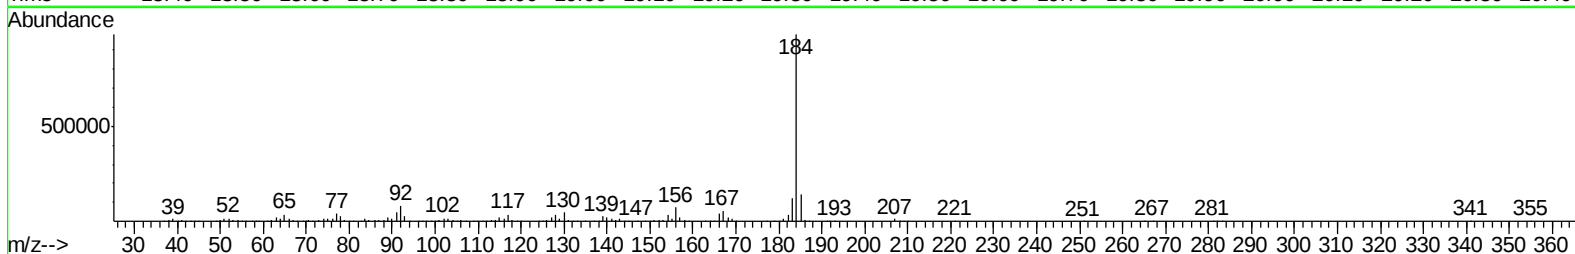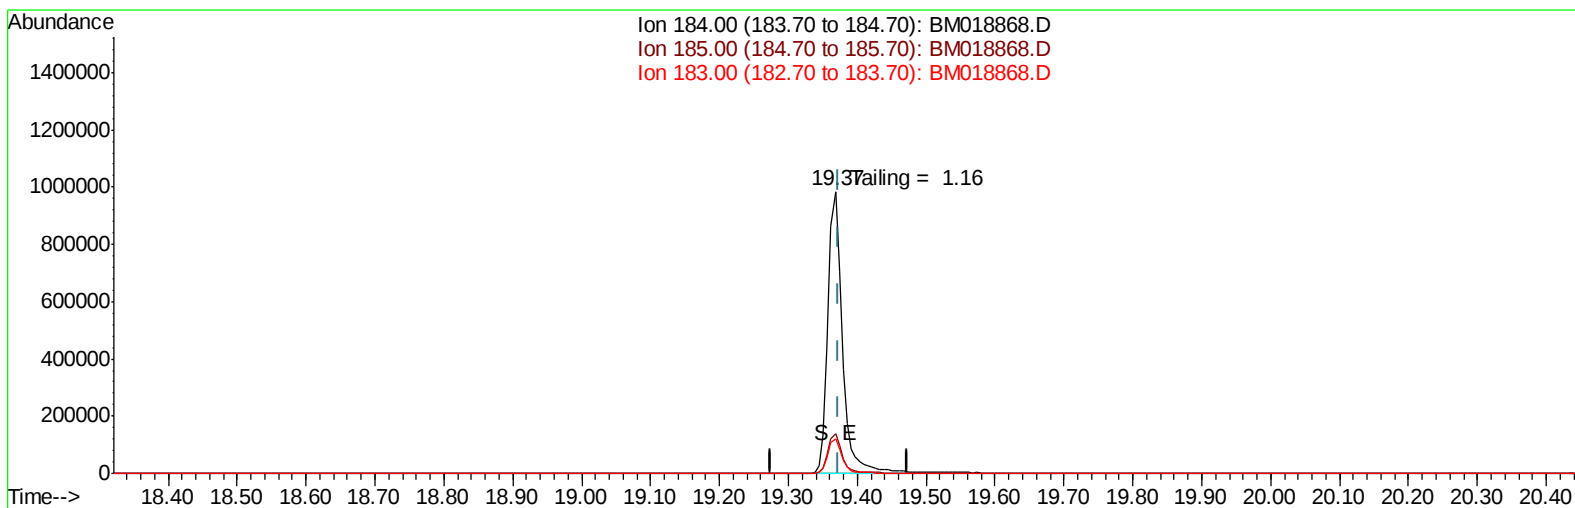

TIC: BM018868.D

(77) Benzidine

19.368min (-0.006) 39627.50ng

response 1416346

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	14.13
183.00	12.10	12.19
0.00	0.00	0.00