


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021919\
 Data File : BM018852.D
 Acq On : 19 Feb 2019 11:07
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 11 16:02:12 2019

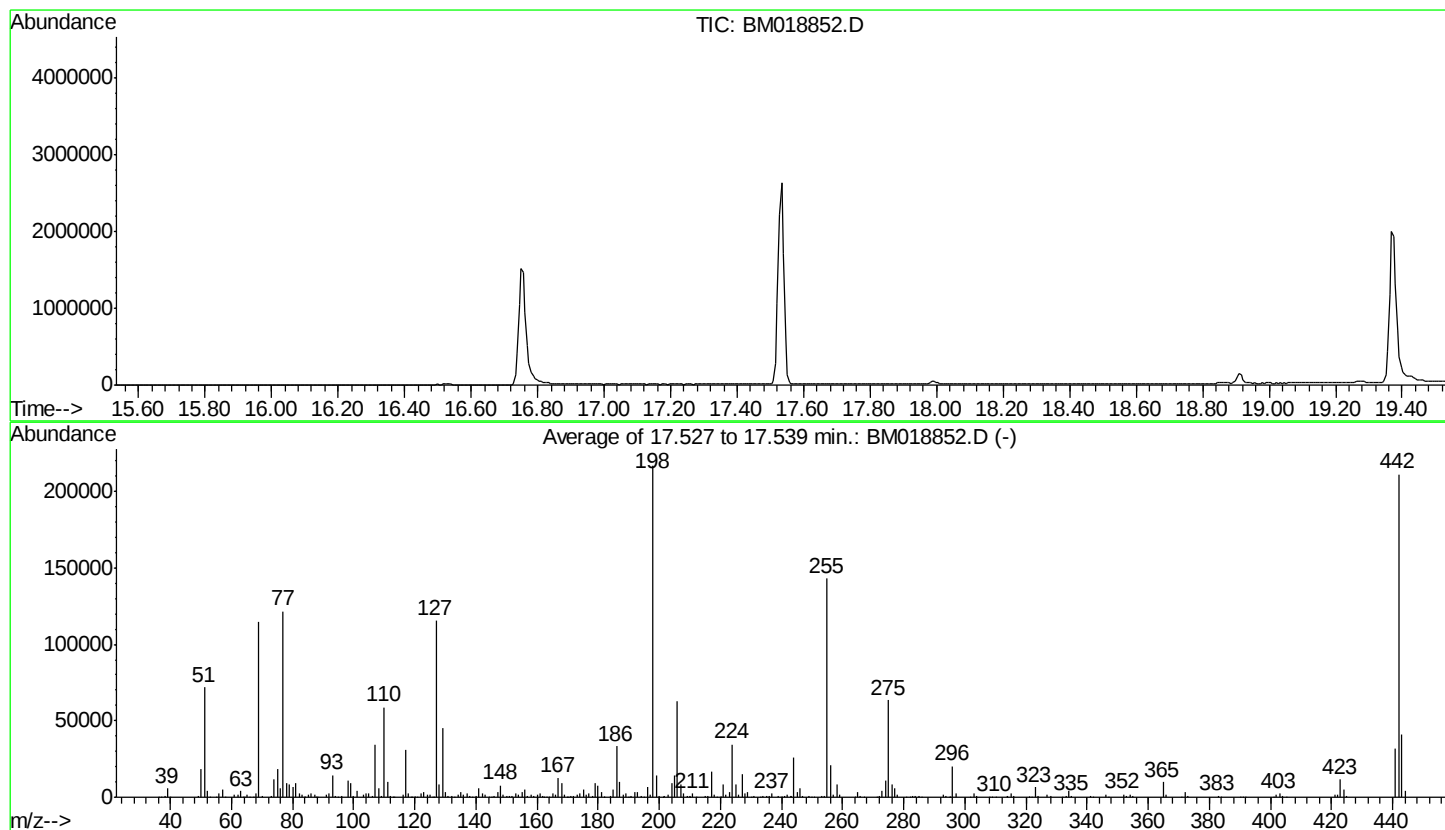

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	71714	PASS
68	69	0.00	2	2.0	2271	PASS
69	198	0.00	100	53.0	114886	PASS
70	69	0.00	2	0.6	637	PASS
127	198	10	80	53.3	115514	PASS
197	198	0.00	2	0.7	1431	PASS
198	198	100	100	100.0	216874	PASS
199	198	5	9	6.5	14011	PASS
275	198	10	60	29.3	63490	PASS
365	198	1	100	4.6	10014	PASS
441	198	0.01	100	14.6	31744	PASS
442	198	50	100	97.5	211370	PASS
443	442	15	24	19.3	40738	PASS