


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021919\  
 Data File : BM018868.D  
 Acq On : 19 Feb 2019 23:15  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM021119.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Feb 11 16:02:12 2019

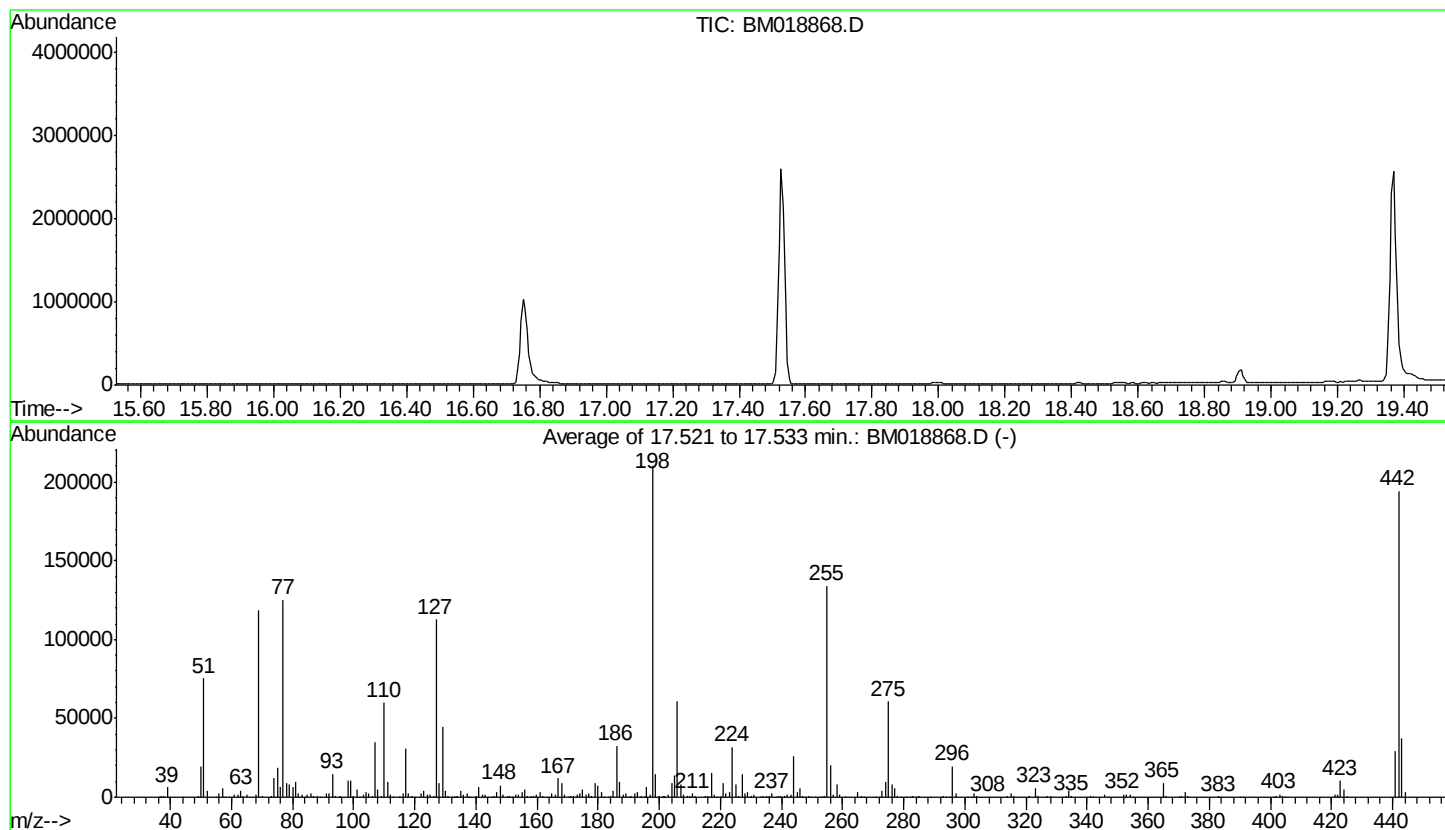

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2448

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 35.7      | 75184   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 2041    | PASS             |
| 69          | 198          | 0.00         | 100          | 56.5      | 118792  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.7       | 807     | PASS             |
| 127         | 198          | 10           | 80           | 53.6      | 112746  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 1366    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 210325  | PASS             |
| 199         | 198          | 5            | 9            | 7.1       | 14903   | PASS             |
| 275         | 198          | 10           | 60           | 28.8      | 60634   | PASS             |
| 365         | 198          | 1            | 100          | 4.3       | 9108    | PASS             |
| 441         | 198          | 0.01         | 100          | 14.0      | 29502   | PASS             |
| 442         | 198          | 50           | 100          | 92.3      | 194168  | PASS             |
| 443         | 442          | 15           | 24           | 19.4      | 37688   | PASS             |