


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022023\
 Data File : BM038785.D
 Acq On : 20 Feb 2023 13:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 21 02:04:34 2023

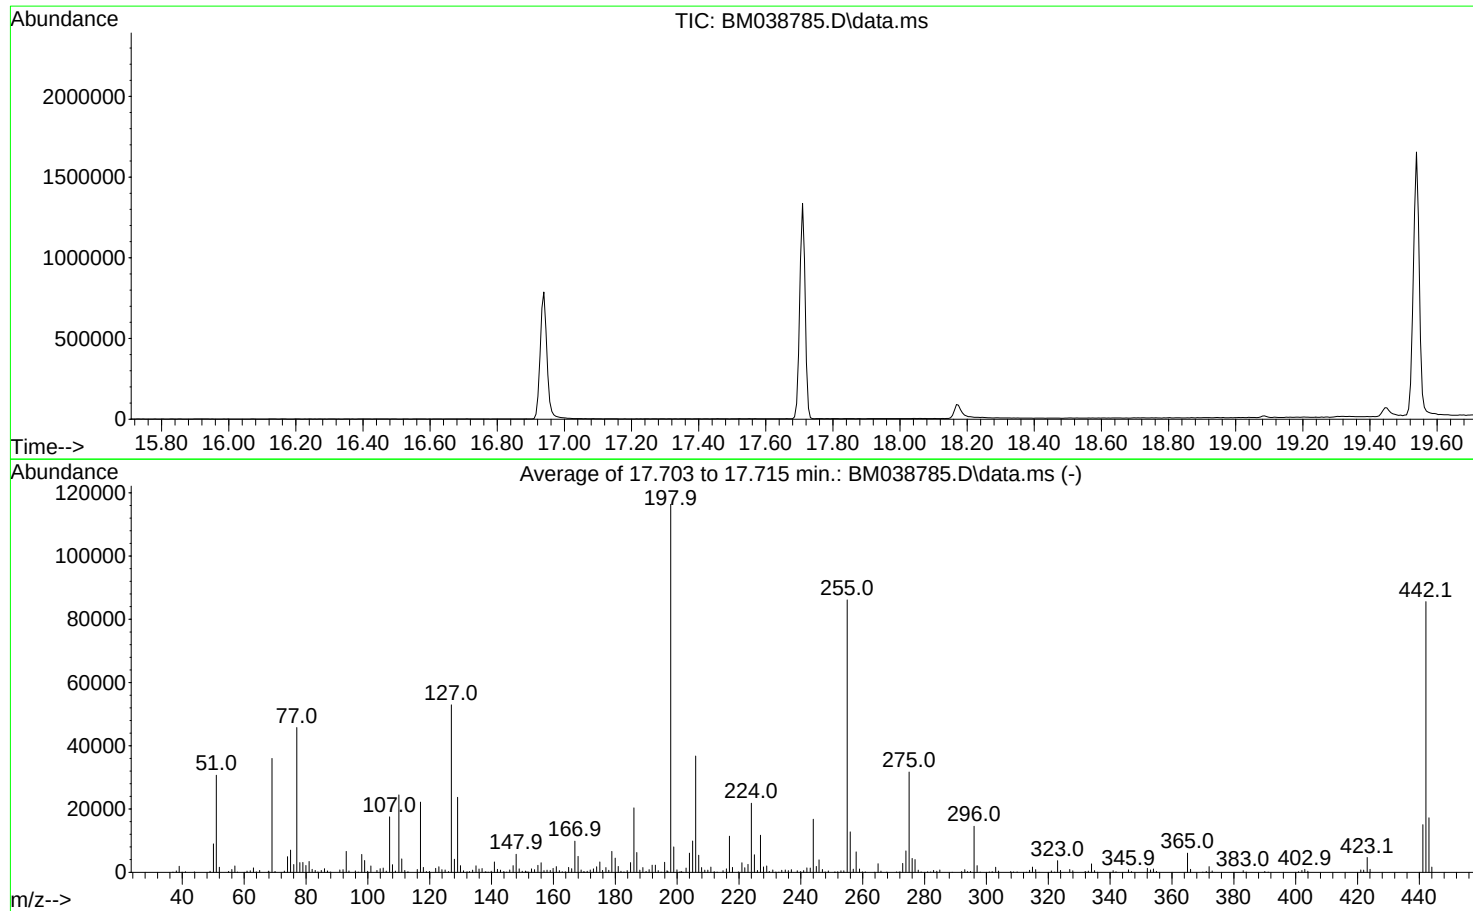




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	30688	PASS
68	69	0.00	2	1.0	368	PASS
69	198	0.00	100	30.9	36005	PASS
70	69	0.00	2	0.8	278	PASS
127	198	10	80	45.5	52963	PASS
197	198	0.00	2	0.4	480	PASS
198	198	100	100	100.0	116333	PASS
199	198	5	9	6.9	8028	PASS
275	198	10	60	27.2	31688	PASS
365	198	1	100	5.2	6058	PASS
441	198	0.01	100	12.9	15041	PASS
442	442	50	100	100.0	85573	PASS
443	442	15	24	20.1	17221	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022023\
Data File : BM038785.D
Acq On : 20 Feb 2023 13:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 21 04:28:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 21 02:04:34 2023
Response via : Initial Calibration

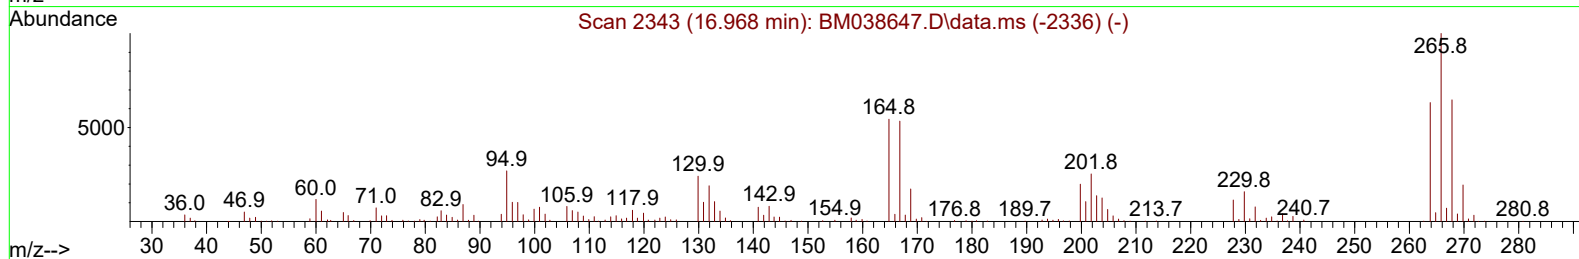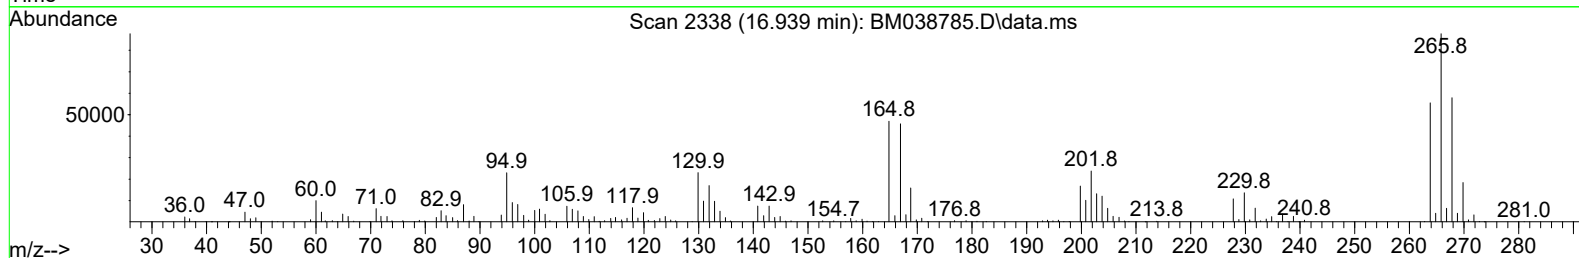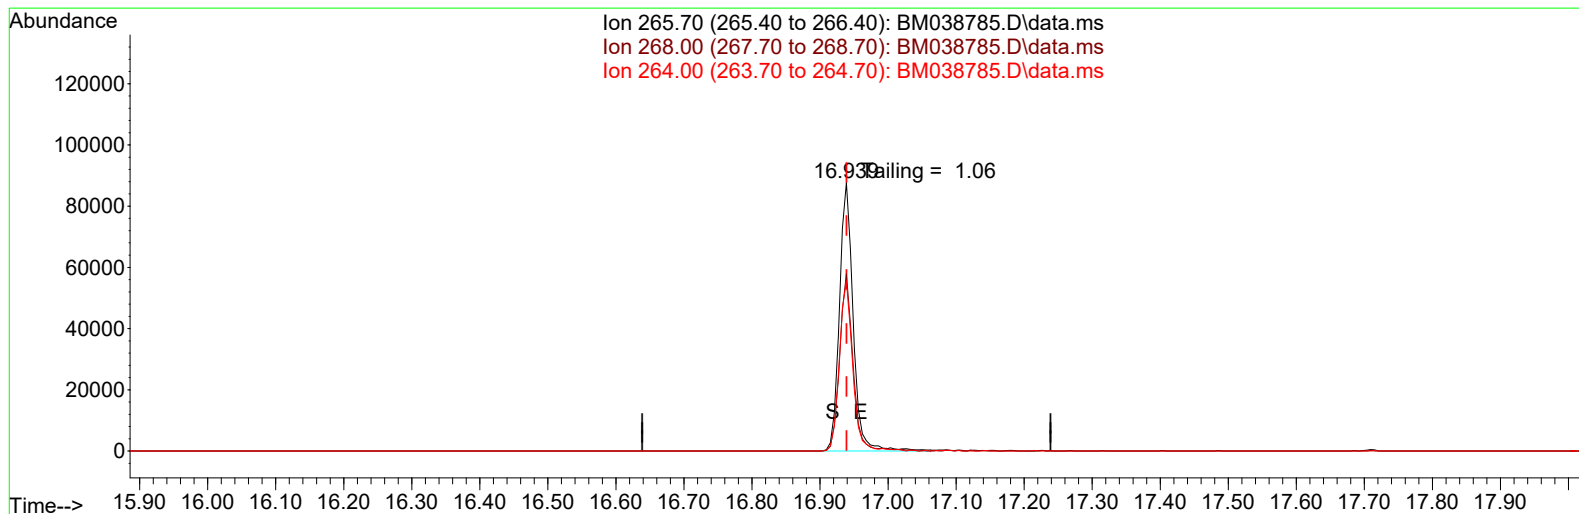

TIC: BM038785.D\data.ms

(70) Pentachlorophenol (C)

16.939min (+ 0.000) 0.00 ng




response 121837

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	66.02
264.00	63.30	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022023\
Data File : BM038785.D
Acq On : 20 Feb 2023 13:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 21 04:28:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 21 02:04:34 2023
Response via : Initial Calibration

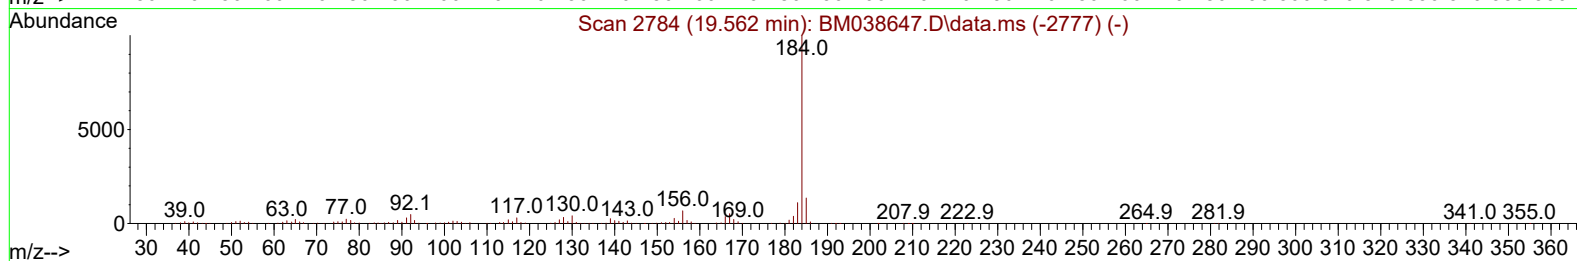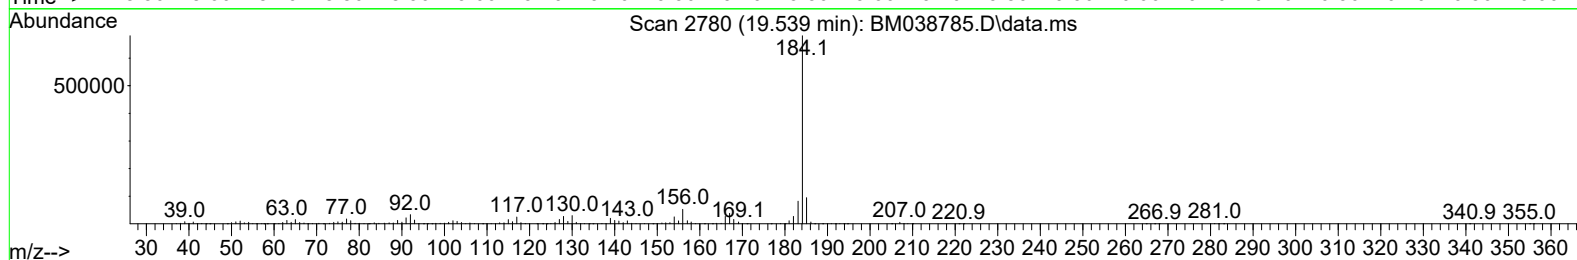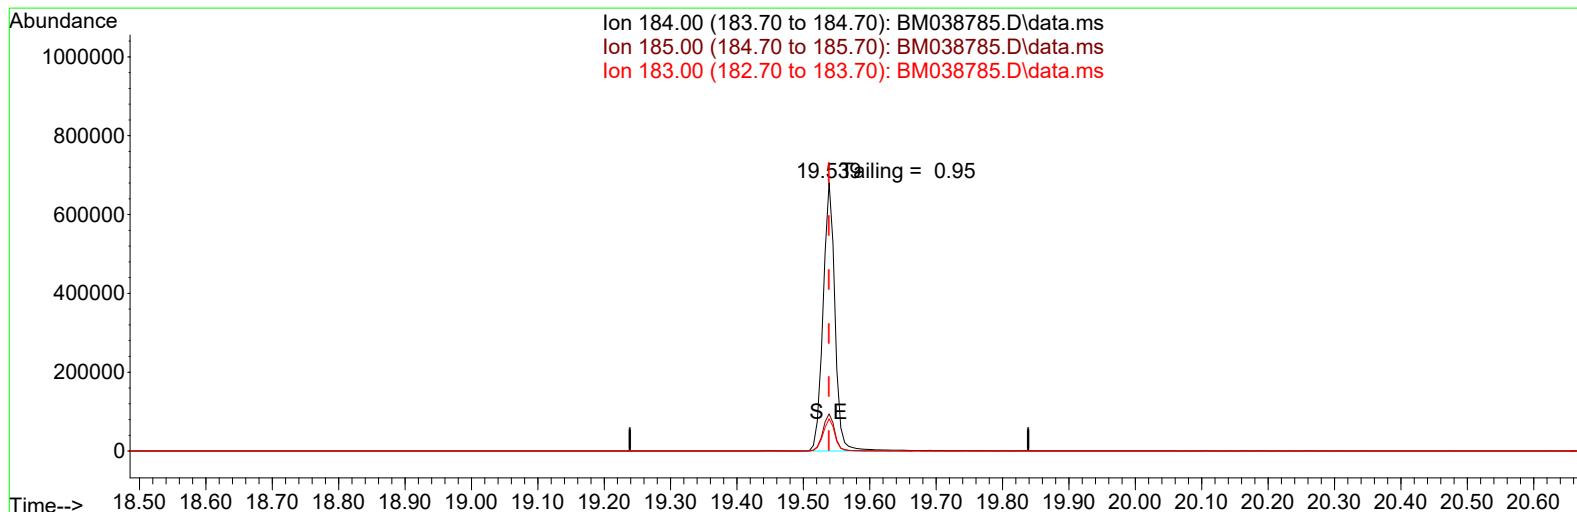

TIC: BM038785.D\data.ms

(77) Benzidine

19.539min (+ 0.000) 22024.06 ng

response 849691

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.88
183.00	11.00	11.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/20/2023	BNA_M	<u>BM038785.D</u>
Compound Name	Response	Retention Time
DDT	926727	20.756
DDD	7004	20.321
DDE	325	19.815
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7329	934056	0.78

Instrument :
BNA_M
ClientSampleId :
DFTPP