
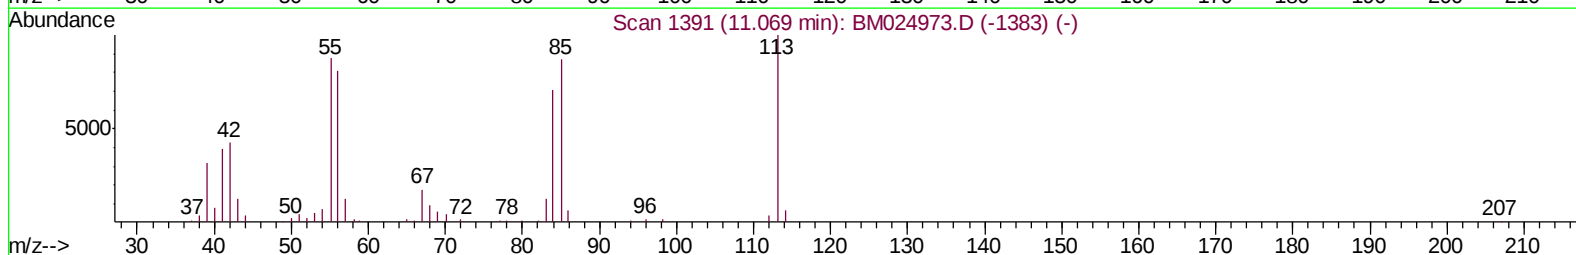
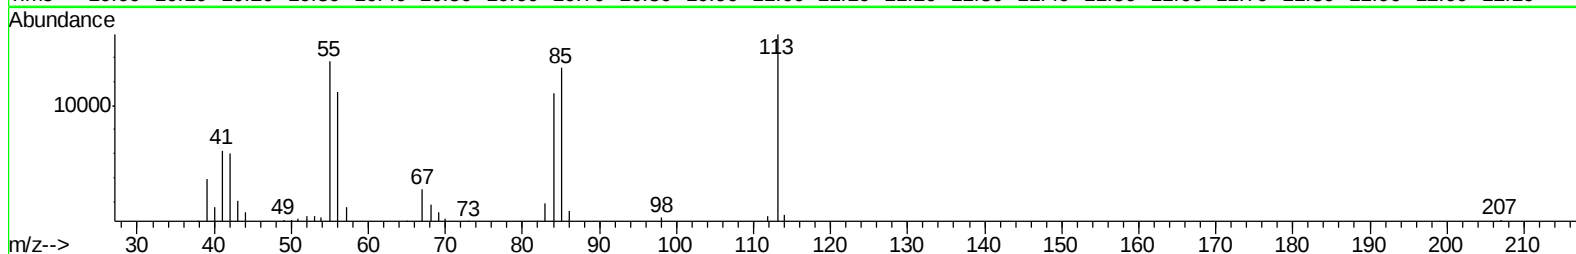


Data File : BM024989.D
Acq On : 21 Feb 2020 16:22
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Feb 22 01:12:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 21 17:03:49 2020
Response via : Initial Calibration

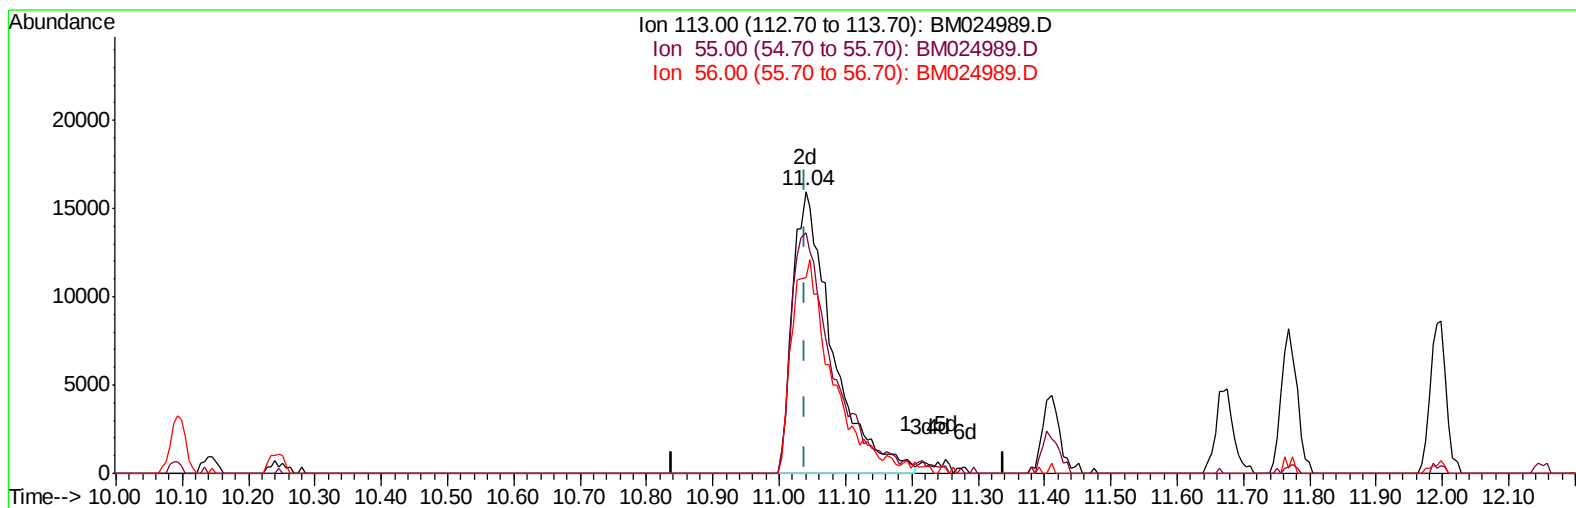

TIC: BM024989.D

(32) Caprolactam

11.039min (0.000) 21.31ng/ul m

response 65925

Ion	Exp%	Act%
113.00	100	100
55.00	107.70	85.63#
56.00	89.90	69.65#
0.00	0.00	0.00