
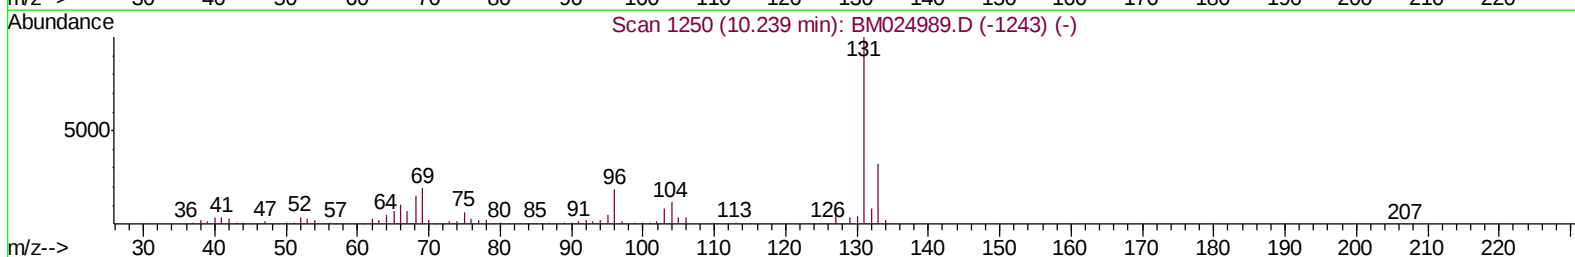
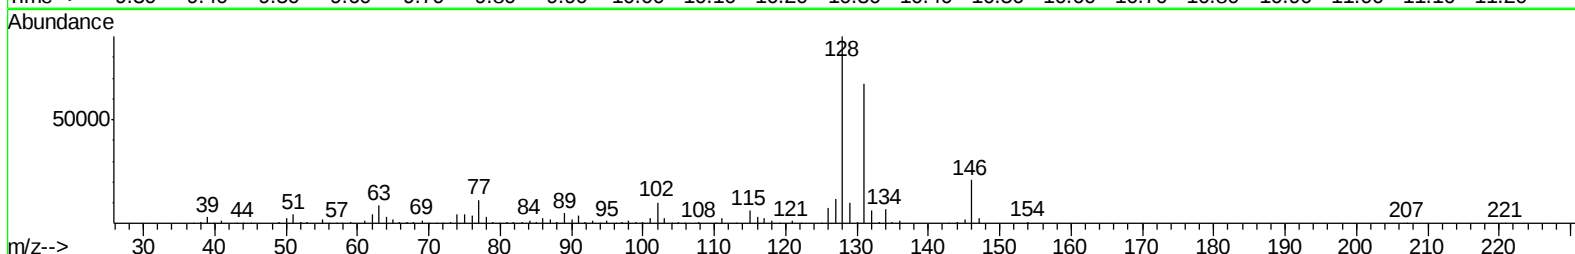


Data File : BM024996.D  
Acq On : 21 Feb 2020 20:46  
Operator : CG/JU  
Sample : L1582-05  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Feb 22 02:16:19 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM020620MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Feb 22 01:15:56 2020  
Response via : Initial Calibration

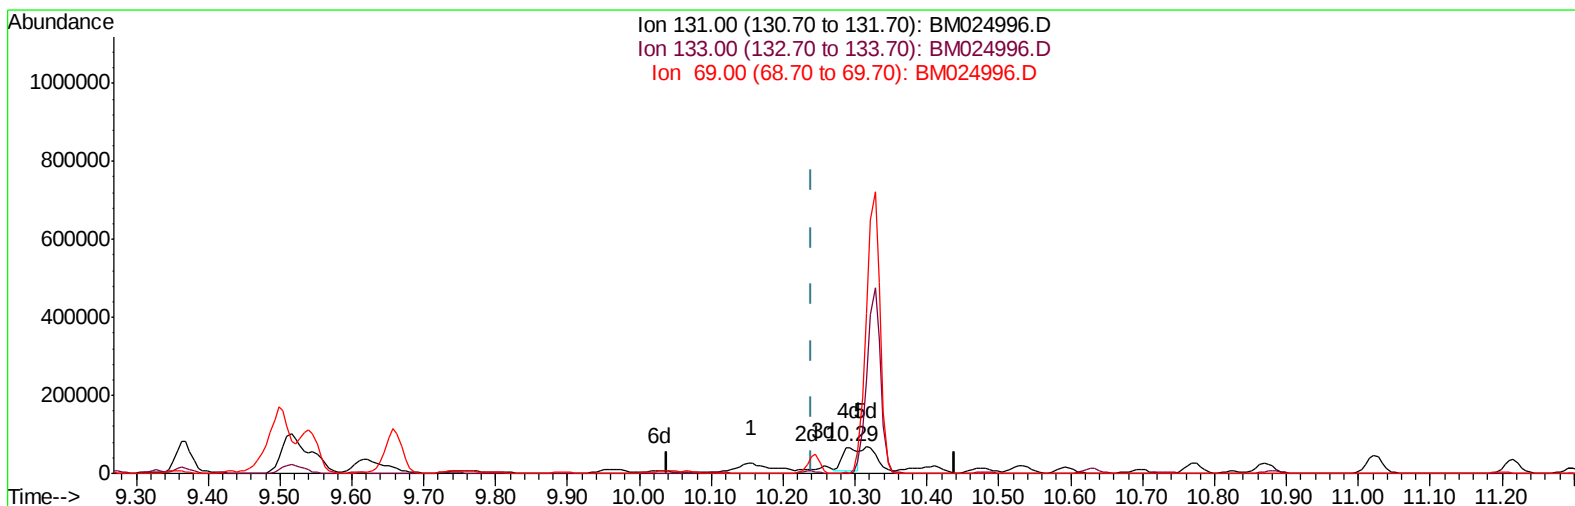

TIC: BM024996.D

(29) 4-Chloroaniline-d4 (S)

10.292min (+0.053) 8.58ng/ul m

response 90669

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 131.00 | 100   | 100   |
| 133.00 | 34.60 | 1.28# |
| 69.00  | 16.20 | 2.44# |
| 0.00   | 0.00  | 0.00  |