
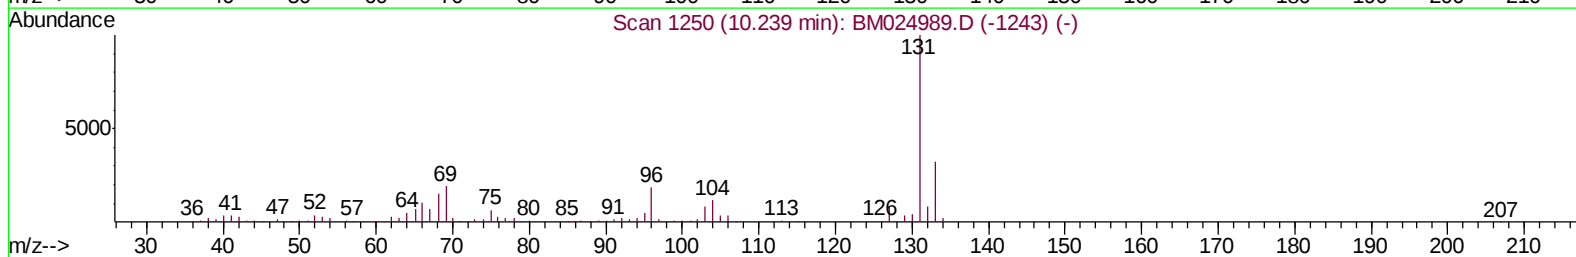
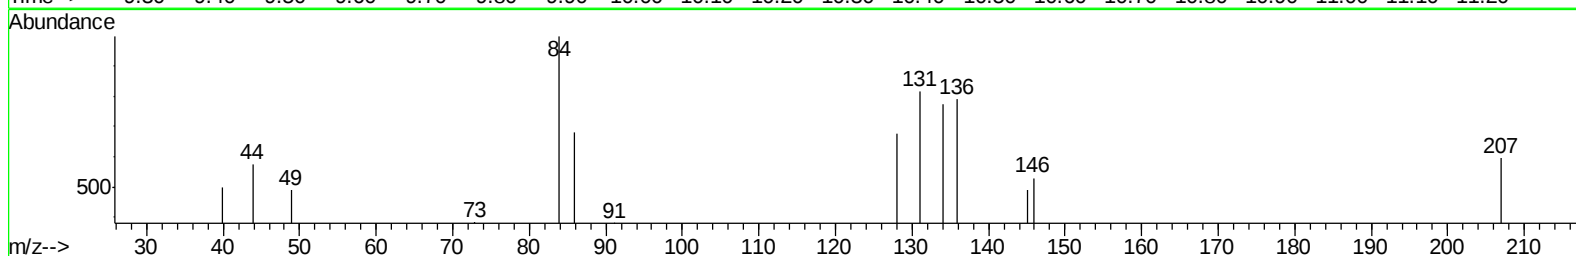


Data File : BM024999.D
Acq On : 21 Feb 2020 22:34
Operator : CG/JU
Sample : L1486-20DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Feb 22 01:19:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 22 01:15:56 2020
Response via : Initial Calibration

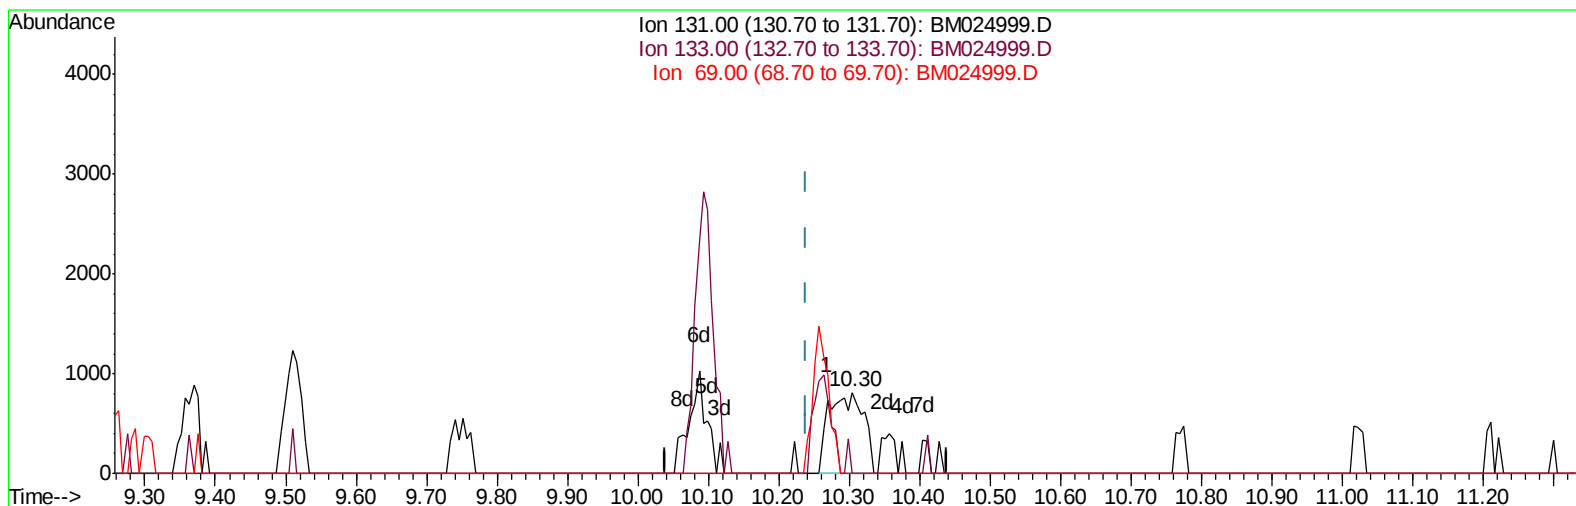

TIC: BM024999.D

(29) 4-Chloroaniline-d4 (S)

10.304min (+0.065) 0.26ng/ul m

response 2748

Ion	Exp%	Act%
131.00	100	100
133.00	34.60	0.00#
69.00	16.20	0.00#
0.00	0.00	0.00