
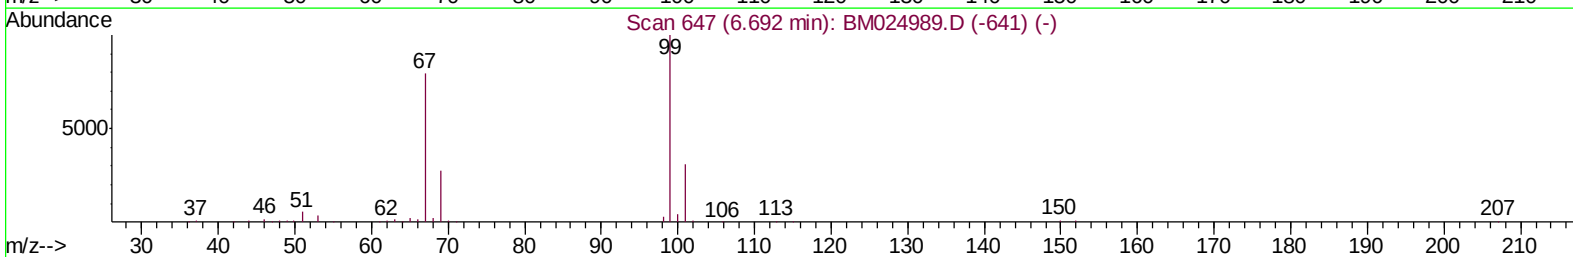
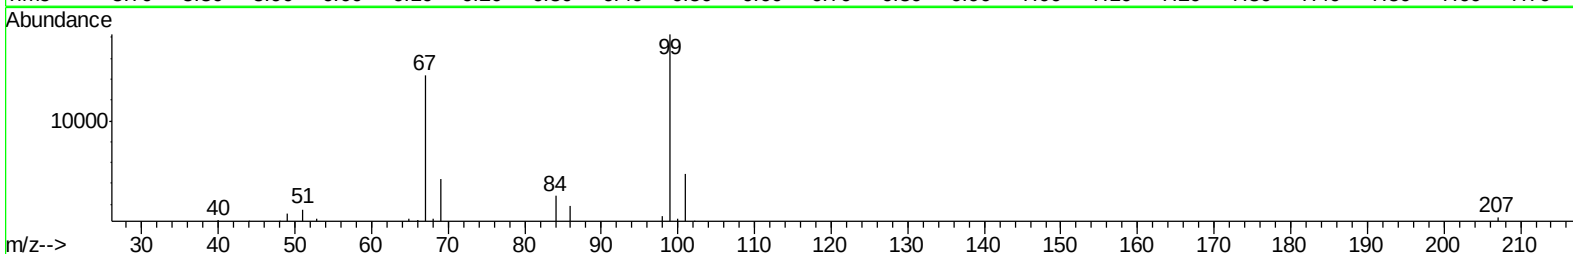


Data File : BM025002.D
Acq On : 22 Feb 2020 00:22
Operator : CG/JU
Sample : L1507-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Feb 22 01:20:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 22 01:15:56 2020
Response via : Initial Calibration

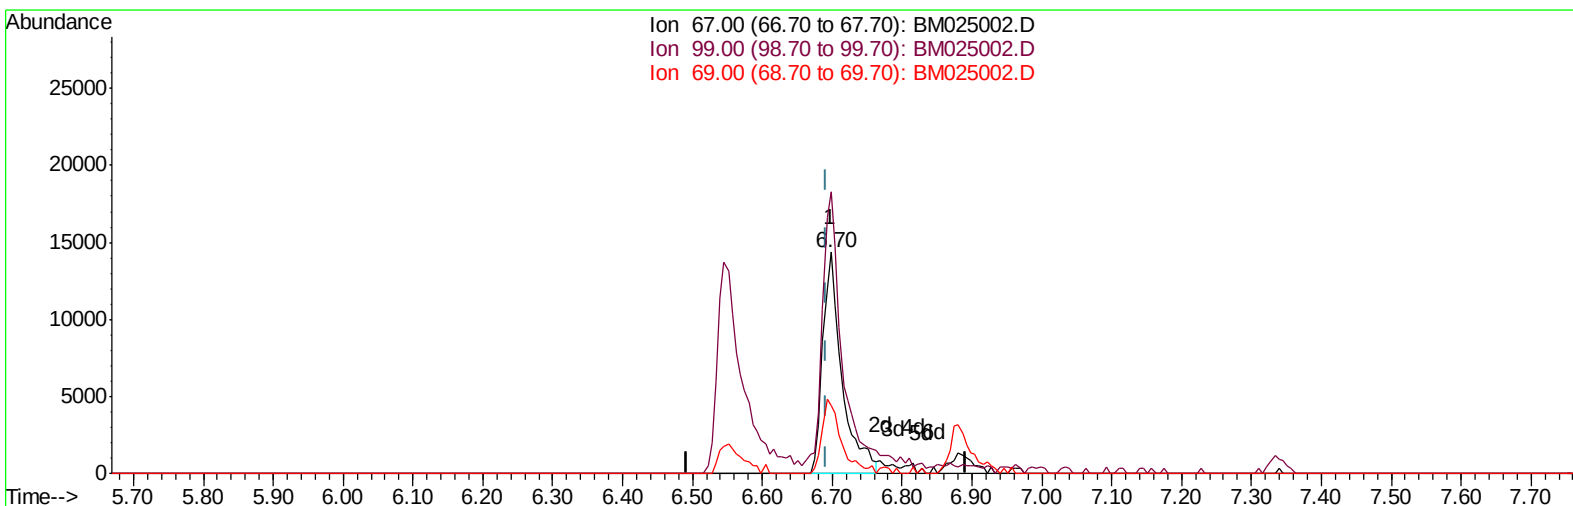

TIC: BM025002.D

(7) Bis-(2-Chloroethyl)ether-d8 (S)

6.698min (+0.006) 5.50ng/ul m

response 27122

Ion	Exp%	Act%
67.00	100	100
99.00	133.80	127.41
69.00	31.80	30.87
0.00	0.00	0.00