
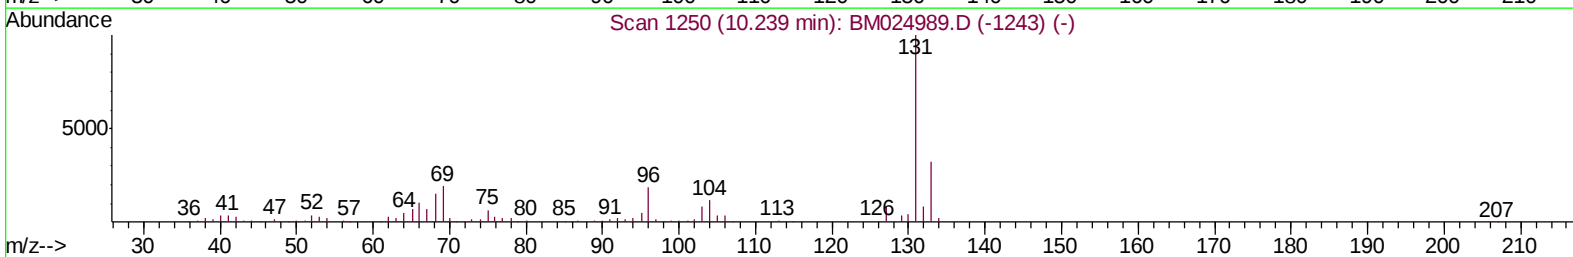
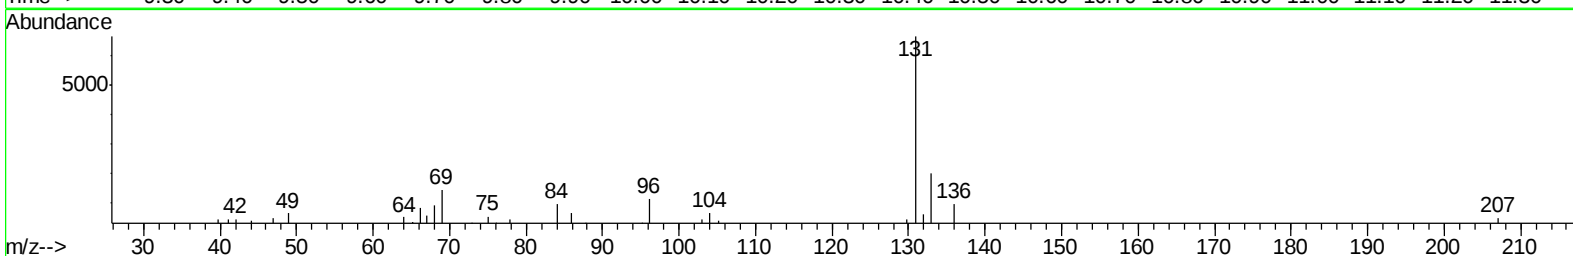


Data File : BM025002.D
Acq On : 22 Feb 2020 00:22
Operator : CG/JU
Sample : L1507-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Feb 22 01:20:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 22 01:15:56 2020
Response via : Initial Calibration

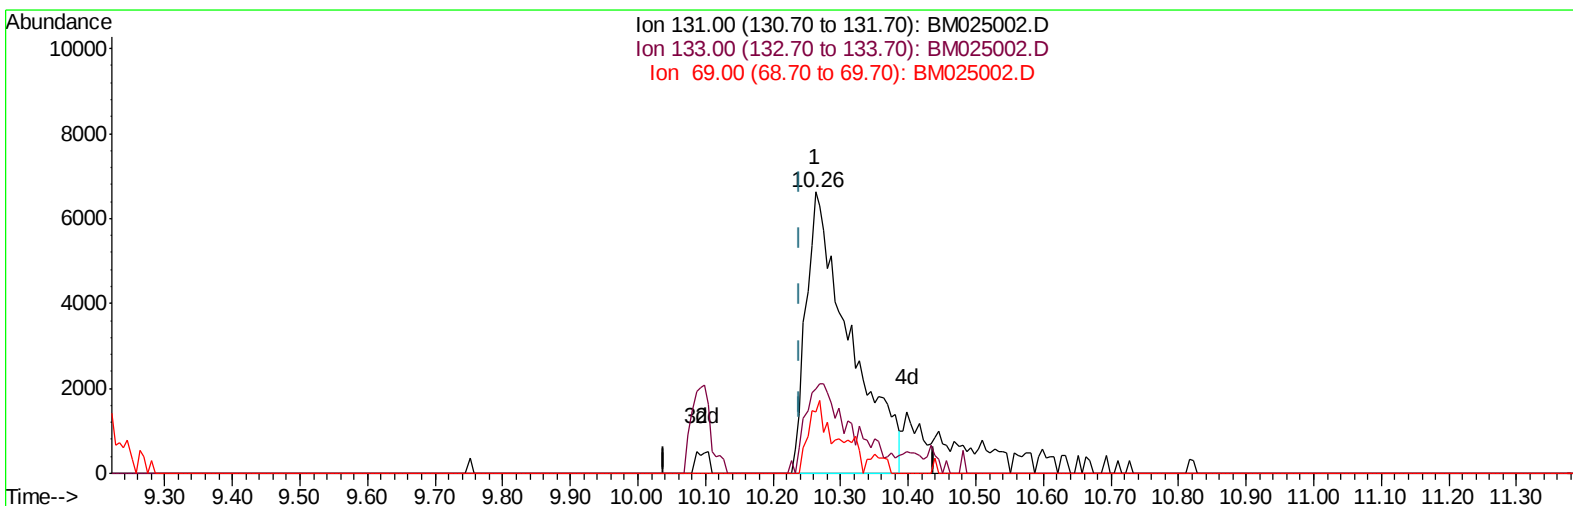

TIC: BM025002.D

(29) 4-Chloroaniline-d4 (S)

10.263min (+0.024) 3.66ng/ul m

response 29473

Ion	Exp%	Act%
131.00	100	100
133.00	34.60	30.03
69.00	16.20	21.81#
0.00	0.00	0.00