
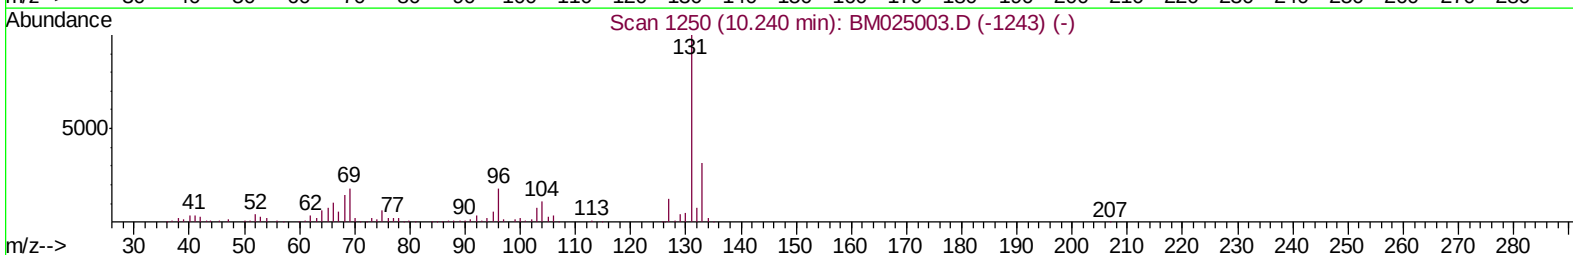
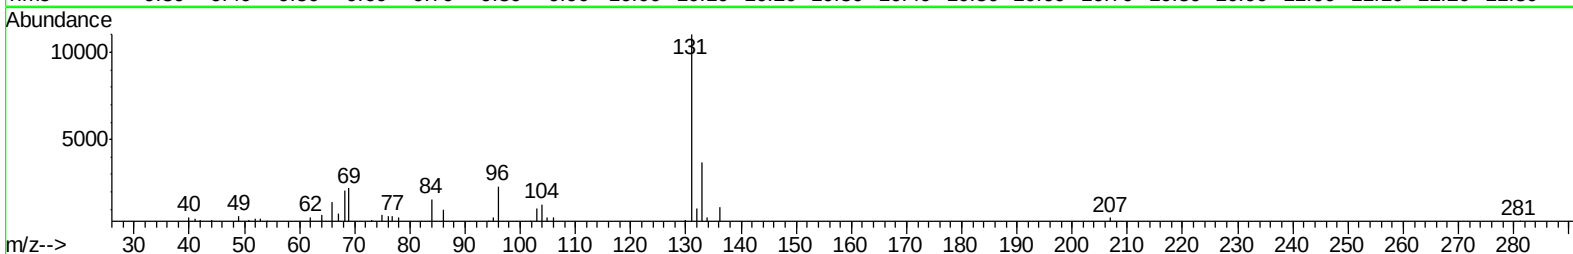


Data File : BM025012.D
Acq On : 22 Feb 2020 06:21
Operator : CG/JU
Sample : L1507-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Feb 24 03:29:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 03:25:45 2020
Response via : Initial Calibration

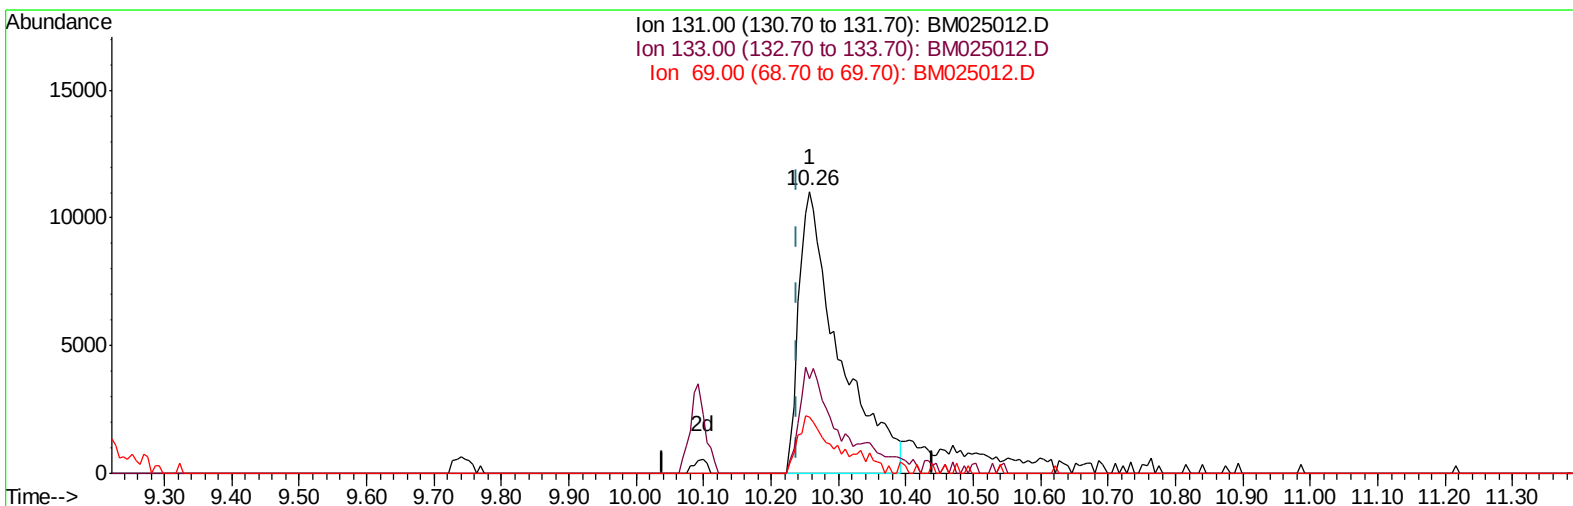

TIC: BM025012.D

(29) 4-Chloroaniline-d4 (S)

10.257min (+0.018) 3.90ng/ul m

response 45774

Ion	Exp%	Act%
131.00	100	100
133.00	34.60	33.60
69.00	16.20	19.94#
0.00	0.00	0.00