
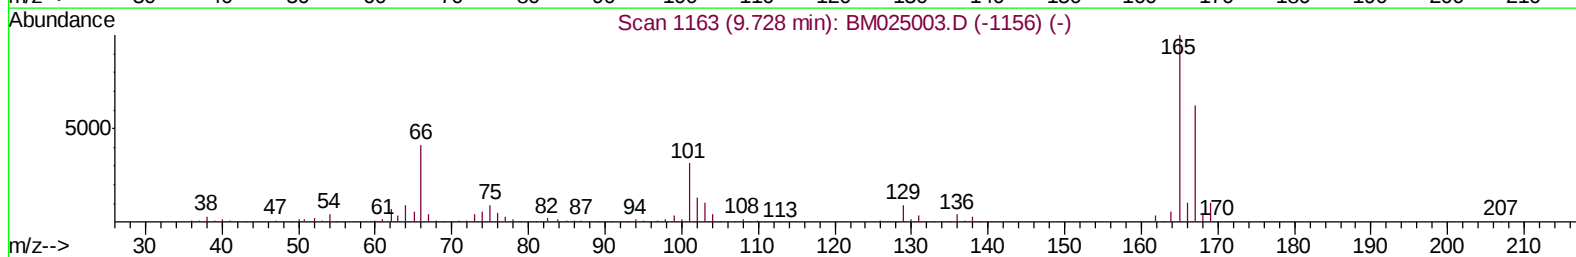
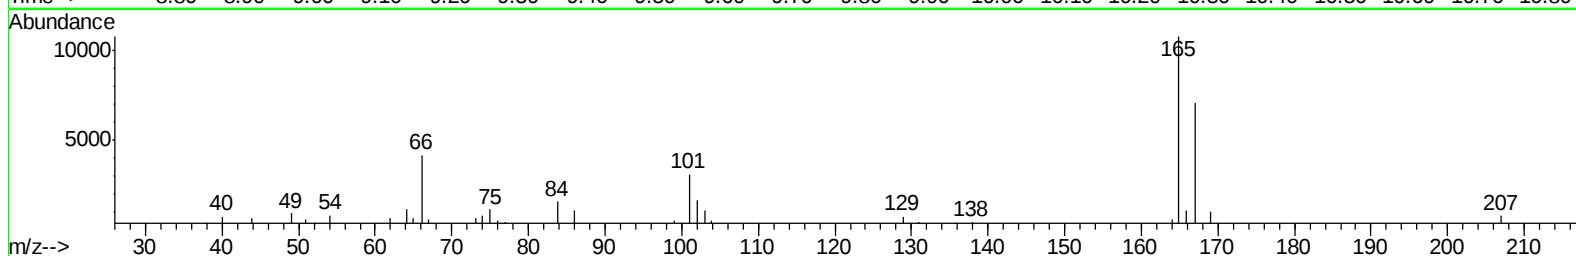


Data File : BM025015.D
Acq On : 22 Feb 2020 08:09
Operator : CG/JU
Sample : L1507-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 24 03:37:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 03:25:45 2020
Response via : Initial Calibration

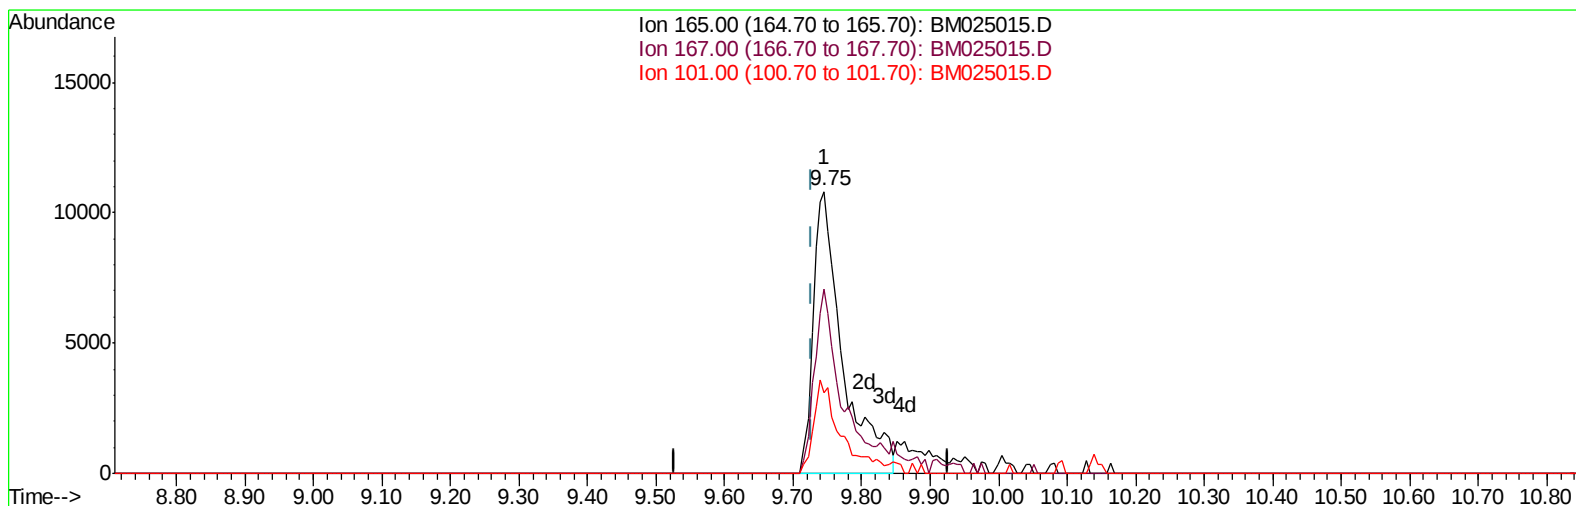

TIC: BM025015.D

(26) 2,4-Dichlorophenol-d3 (S)

9.745min (+0.018) 2.61ng/ul m

response 32274

Ion	Exp%	Act%
165.00	100	100
167.00	66.40	65.56
101.00	30.80	28.57
0.00	0.00	0.00