
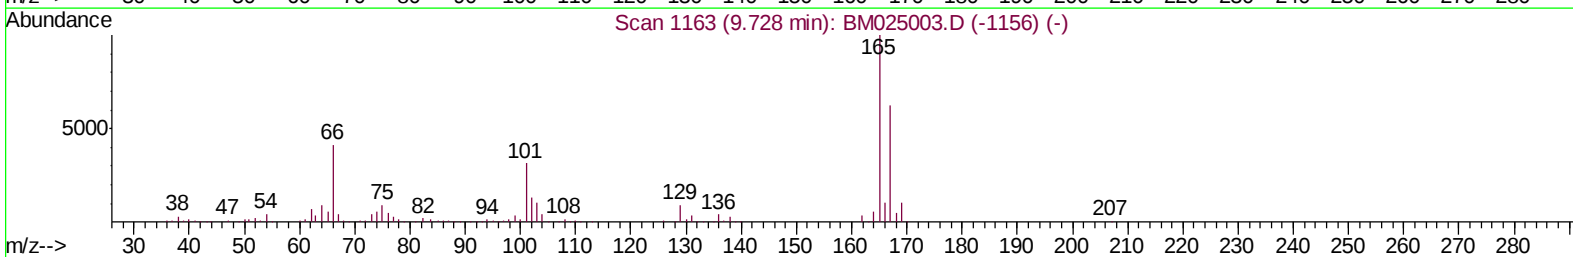
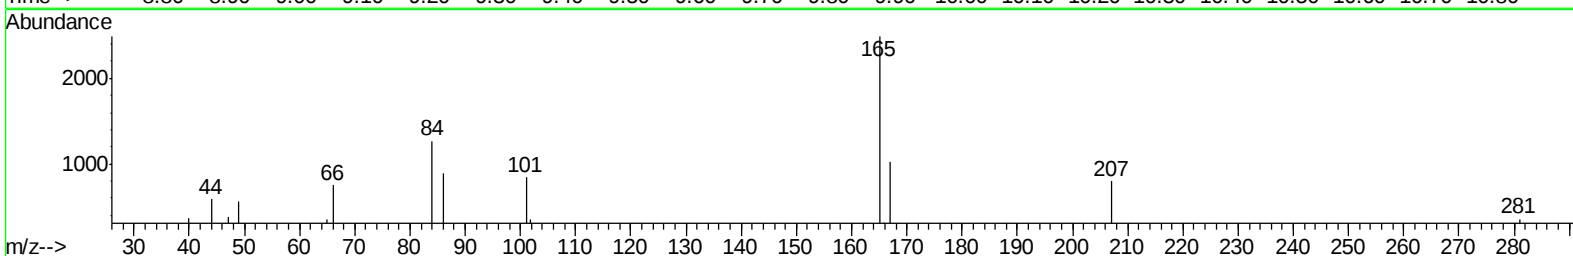


Data File : BM025016.D
Acq On : 22 Feb 2020 08:45
Operator : CG/JU
Sample : L1507-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Feb 24 03:37:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 03:25:45 2020
Response via : Initial Calibration

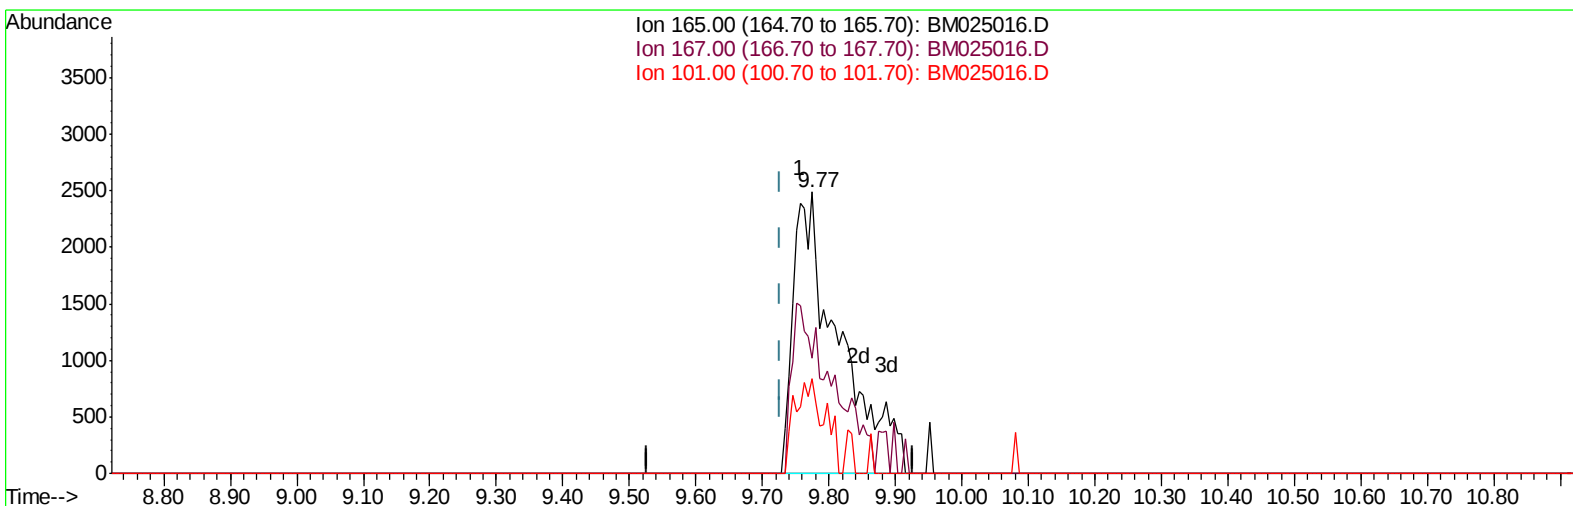

TIC: BM025016.D

(26) 2,4-Dichlorophenol-d3 (S)

9.775min (+0.047) 1.03ng/ul m

response 11948

Ion	Exp%	Act%
165.00	100	100
167.00	66.40	40.92#
101.00	30.80	33.86
0.00	0.00	0.00