
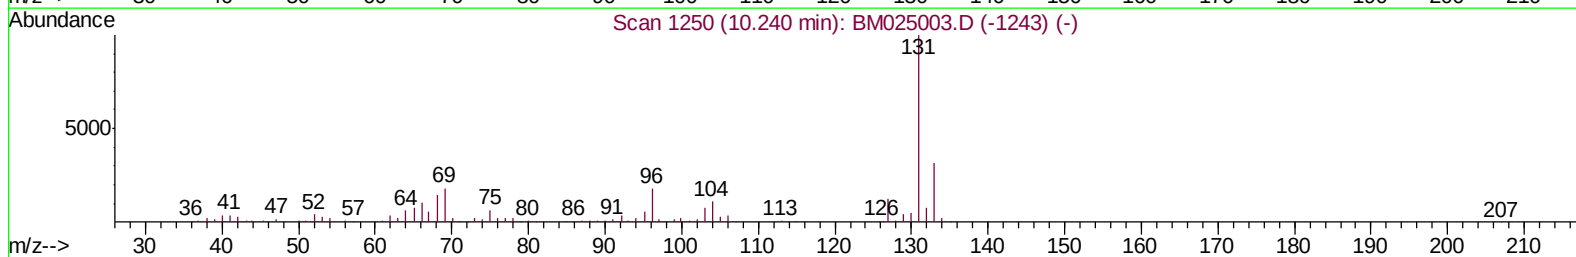
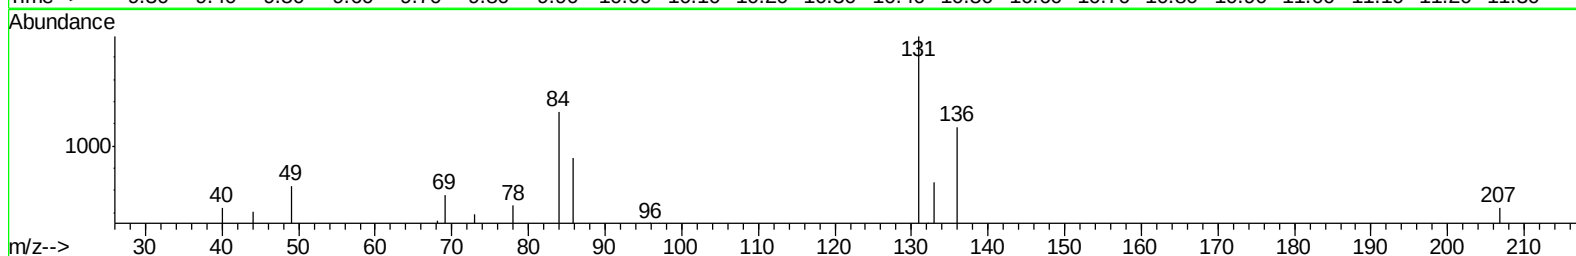


Data File : BM025016.D
Acq On : 22 Feb 2020 08:45
Operator : CG/JU
Sample : L1507-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Feb 24 03:37:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 03:25:45 2020
Response via : Initial Calibration

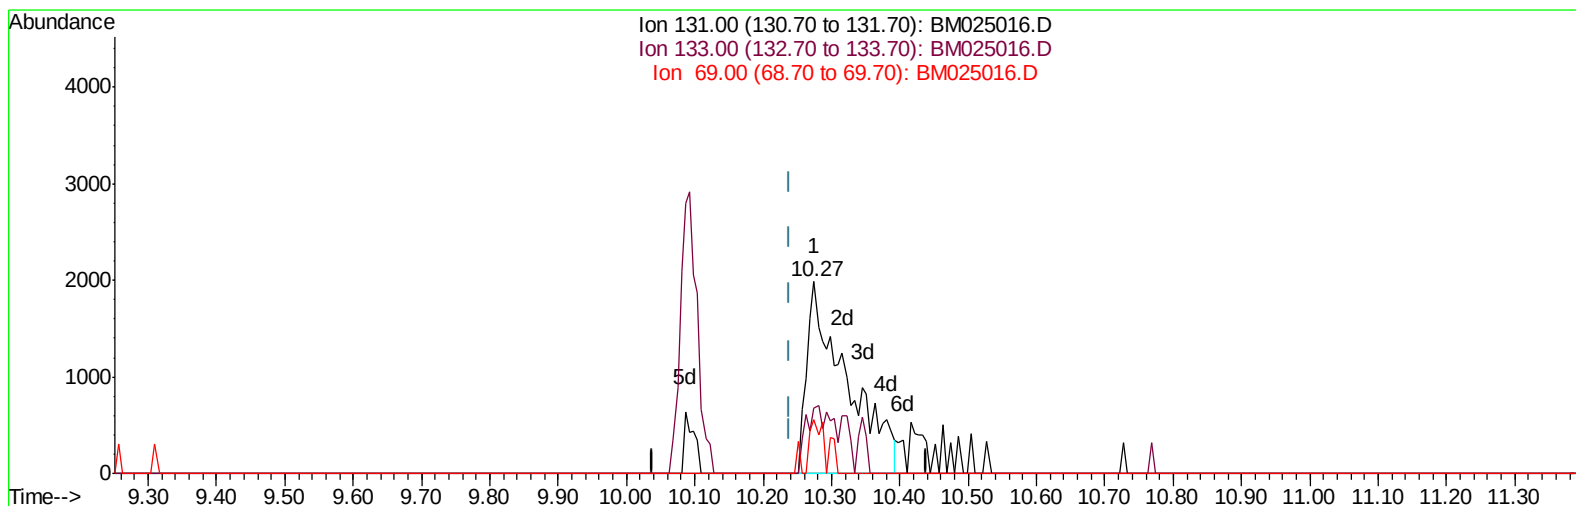

TIC: BM025016.D

(29) 4-Chloroaniline-d4 (S)

10.275min (+0.035) 0.73ng/ul m

response 7932

Ion	Exp%	Act%
131.00	100	100
133.00	34.60	33.89
69.00	16.20	28.15#
0.00	0.00	0.00