
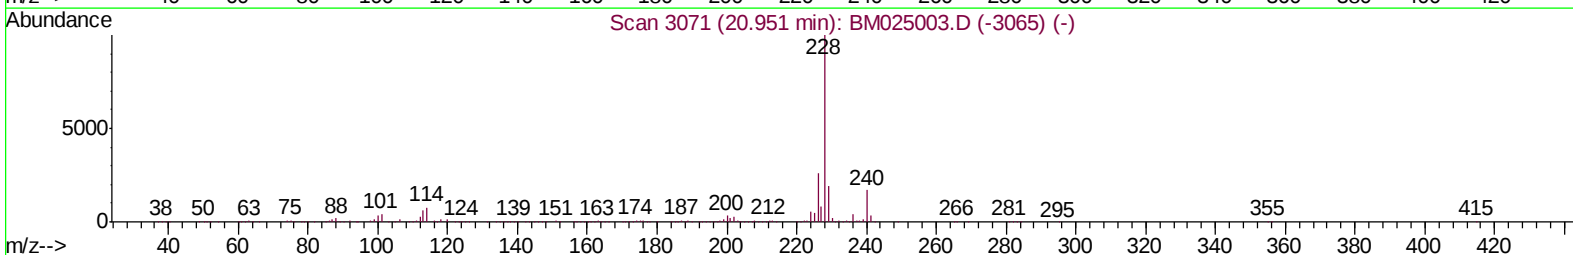
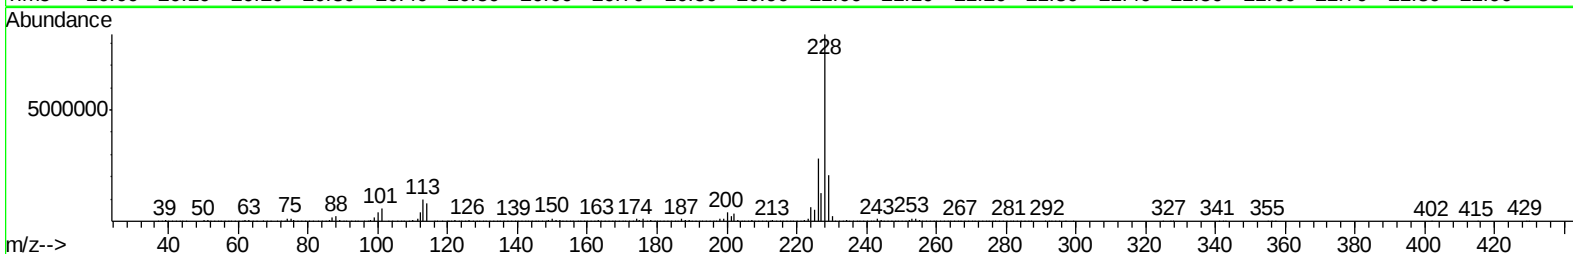


Data File : BM025018.D
Acq On : 22 Feb 2020 09:56
Operator : CG/JU
Sample : L1507-16
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Feb 24 03:37:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 03:25:45 2020
Response via : Initial Calibration

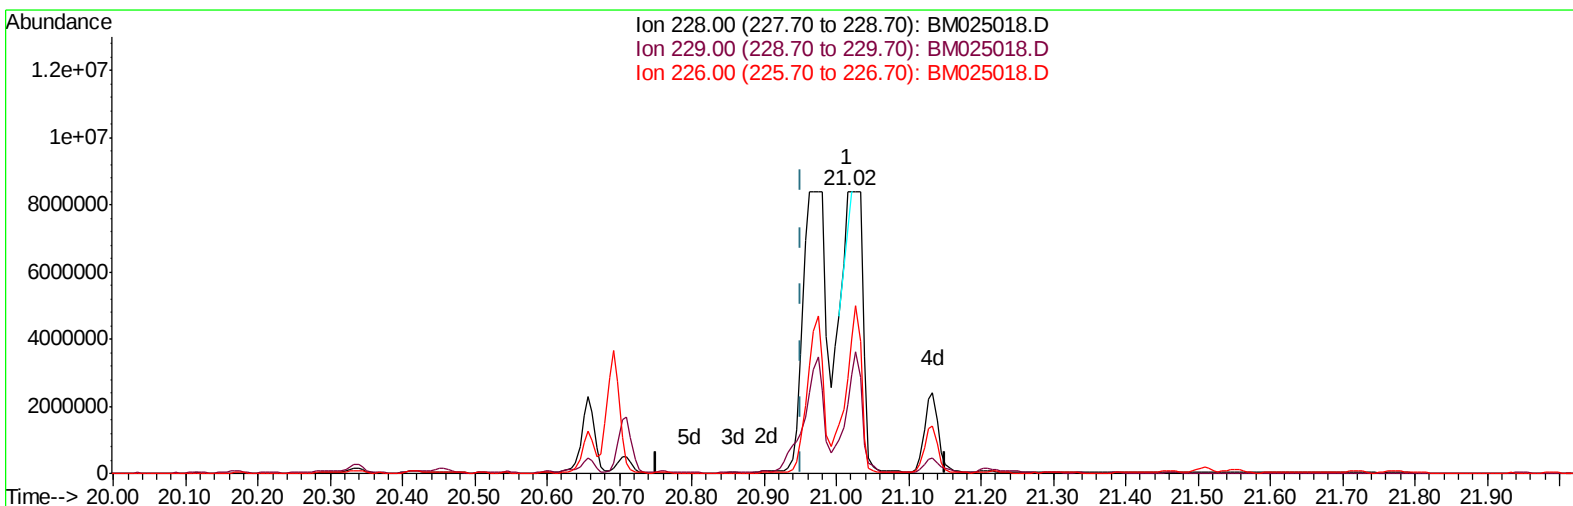

TIC: BM025018.D

(83) Benzo(a)anthracene
21.015min (+0.065) 14.24ng/ul
response 1959269

Ion	Exp%	Act%
228.00	100	100
229.00	19.90	24.70#
226.00	26.00	33.86#
0.00	0.00	0.00