
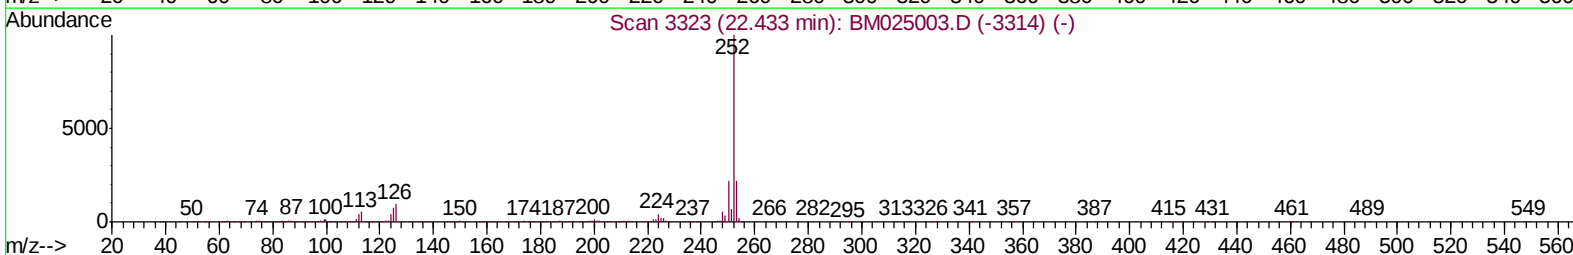
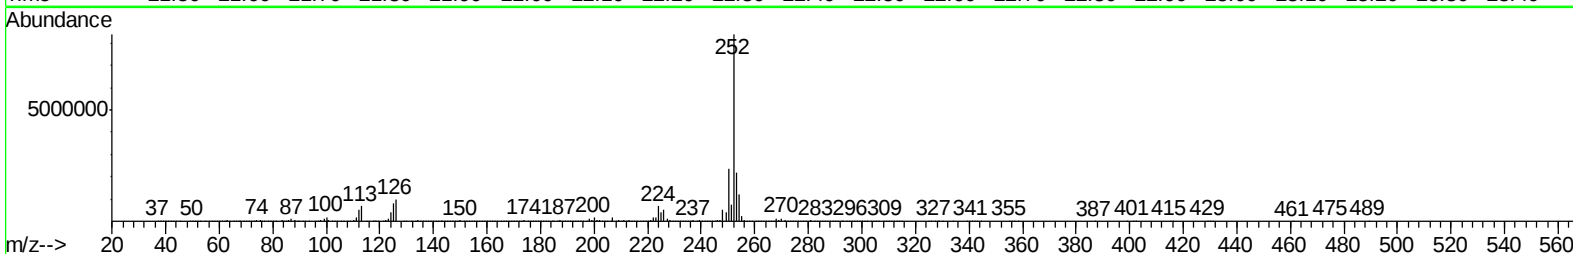


Data File : BM025018.D
Acq On : 22 Feb 2020 09:56
Operator : CG/JU
Sample : L1507-16
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Feb 24 03:37:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 03:25:45 2020
Response via : Initial Calibration

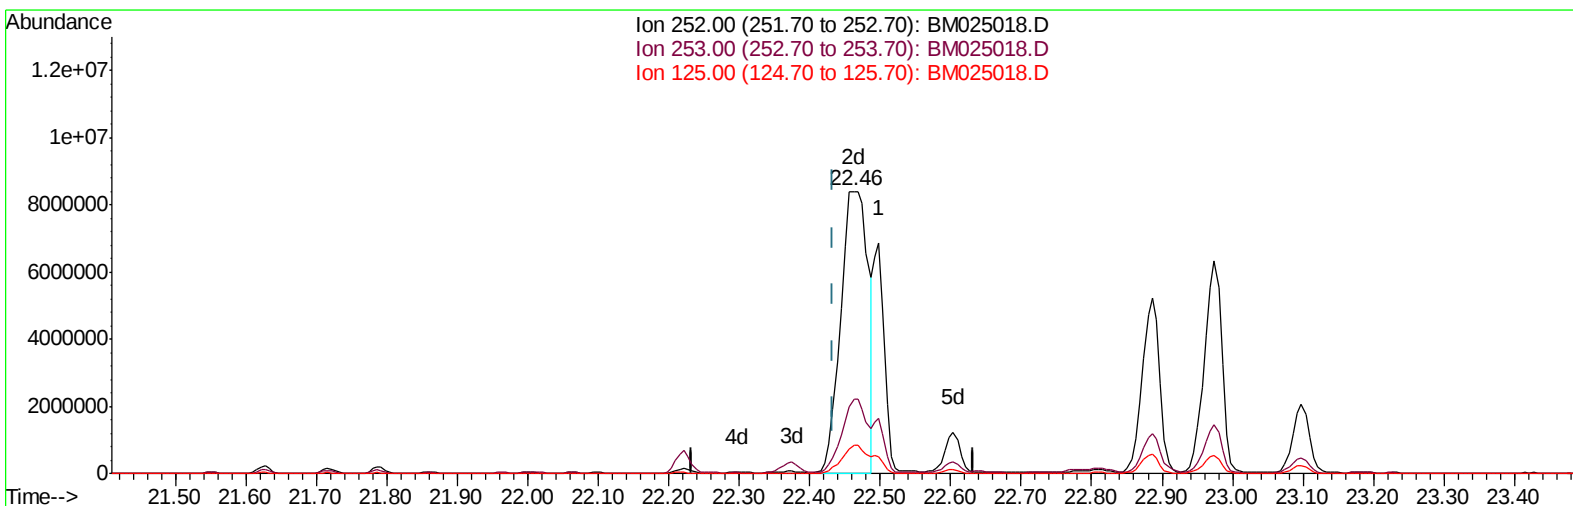

TIC: BM025018.D

(88) Benzo(b)fluoranthene

22.462min (+0.030) 152.40ng/ul m

response 22512748

Ion	Exp%	Act%
252.00	100	100
253.00	21.60	26.21#
125.00	6.40	9.90#
0.00	0.00	0.00