
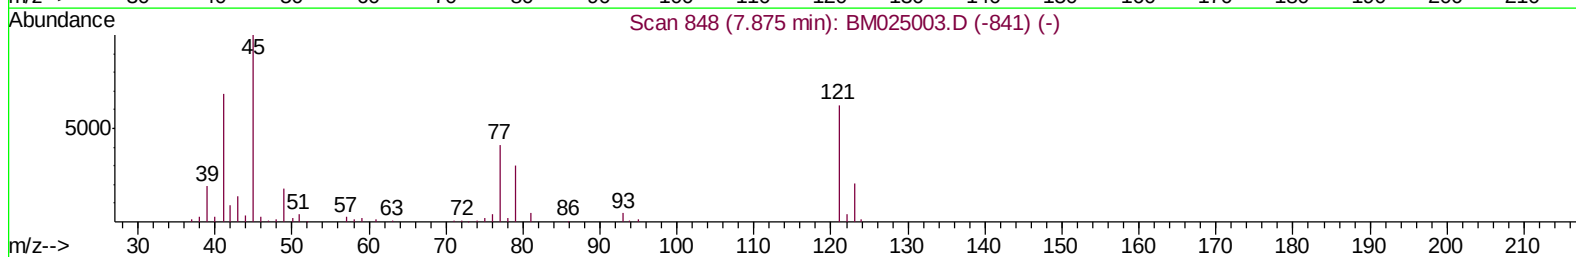
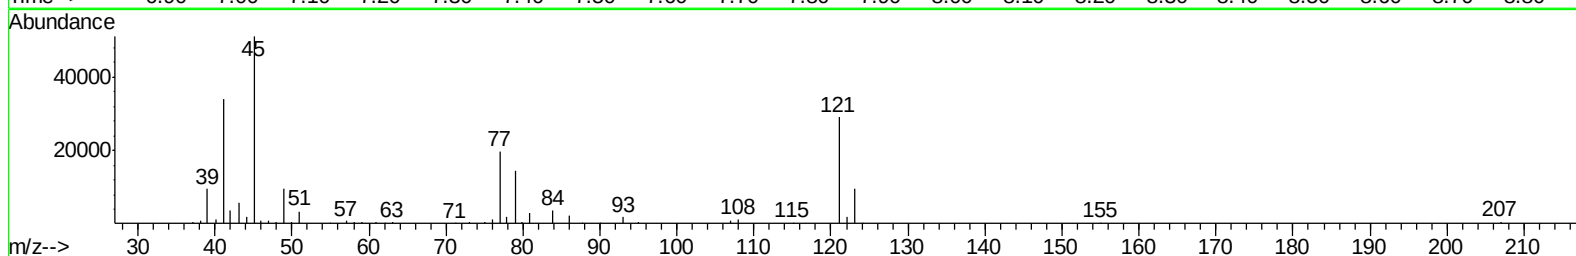


Data File : BM025019.D
Acq On : 22 Feb 2020 10:32
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Feb 24 04:00:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 03:25:45 2020
Response via : Initial Calibration

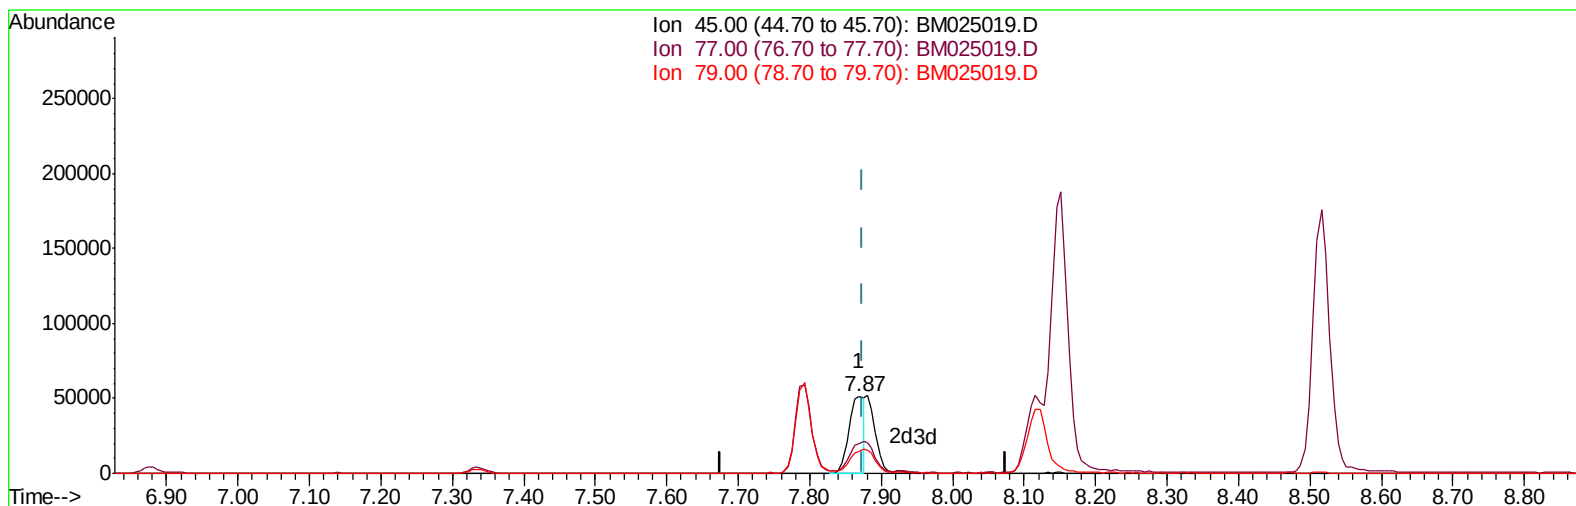

TIC: BM025019.D

(12) 2,2'-oxybis(1-Chloropropane)

7.869min (-0.006) 9.99ng/ul

response 77081

Ion	Exp%	Act%
45.00	100	100
77.00	25.70	38.66#
79.00	17.70	28.45#
0.00	0.00	0.00