
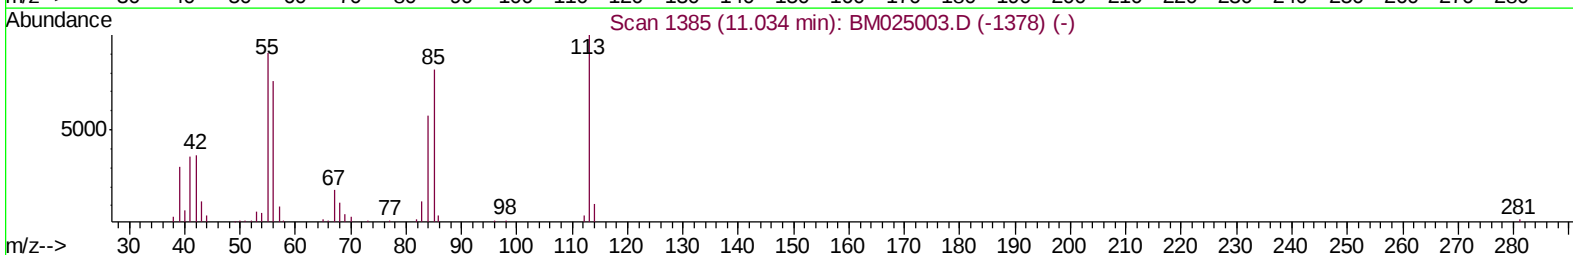
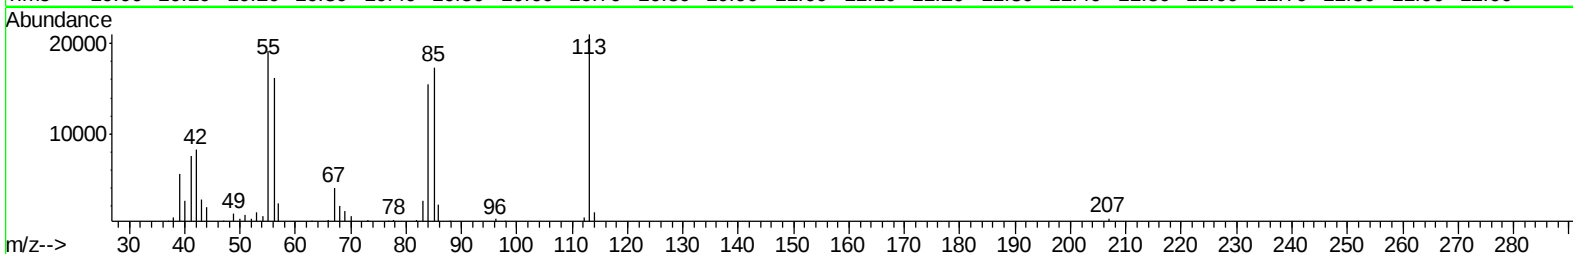


Data File : BM025019.D
Acq On : 22 Feb 2020 10:32
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Feb 24 04:00:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 03:25:45 2020
Response via : Initial Calibration

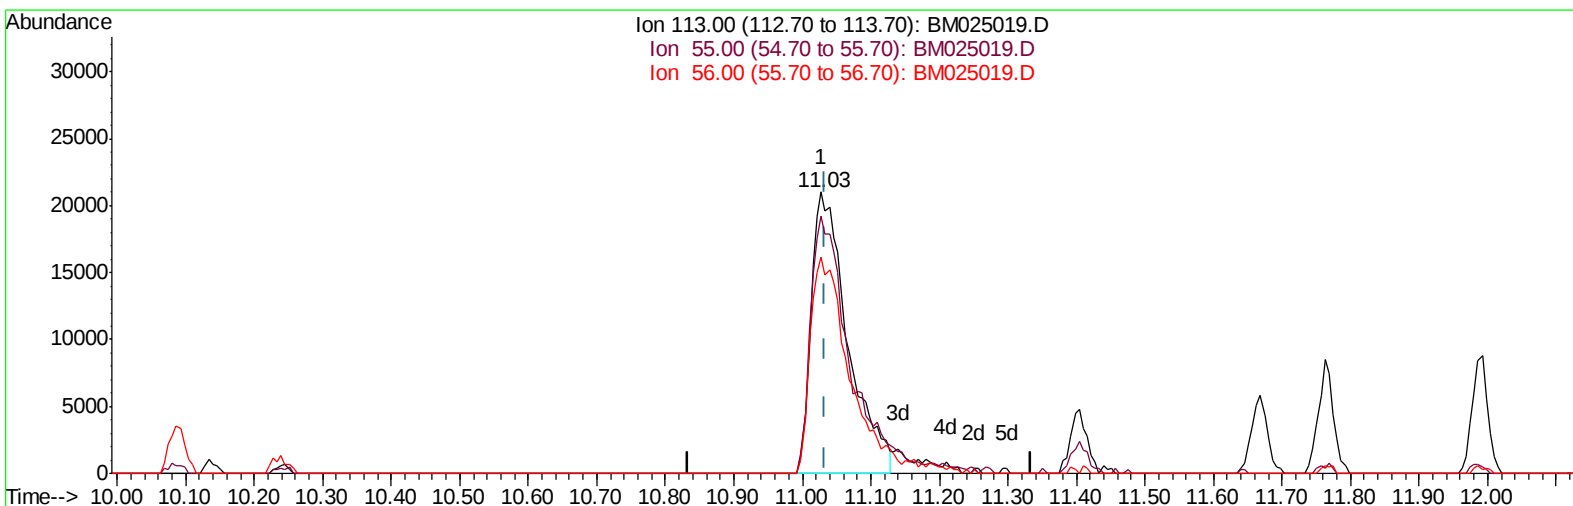

TIC: BM025019.D

(32) Caprolactam

11.027min (-0.006) 23.66ng/ul m

response 77454

Ion	Exp%	Act%
113.00	100	100
55.00	107.70	91.29
56.00	89.90	76.95
0.00	0.00	0.00