
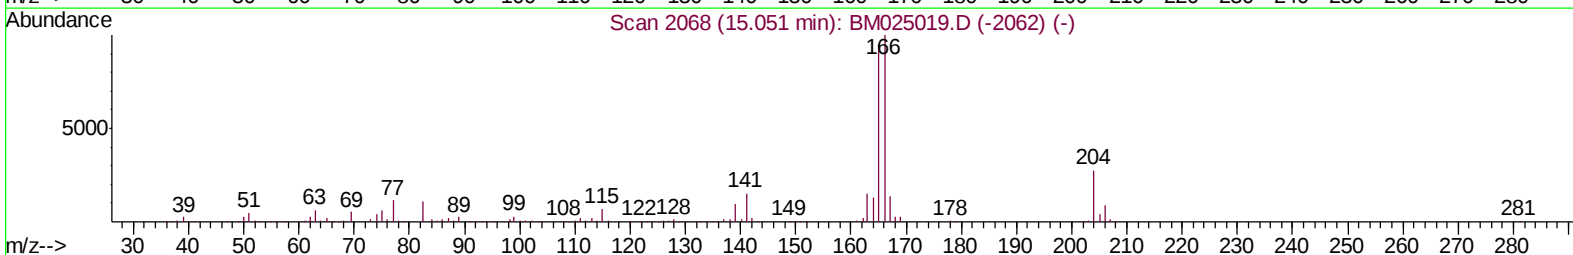
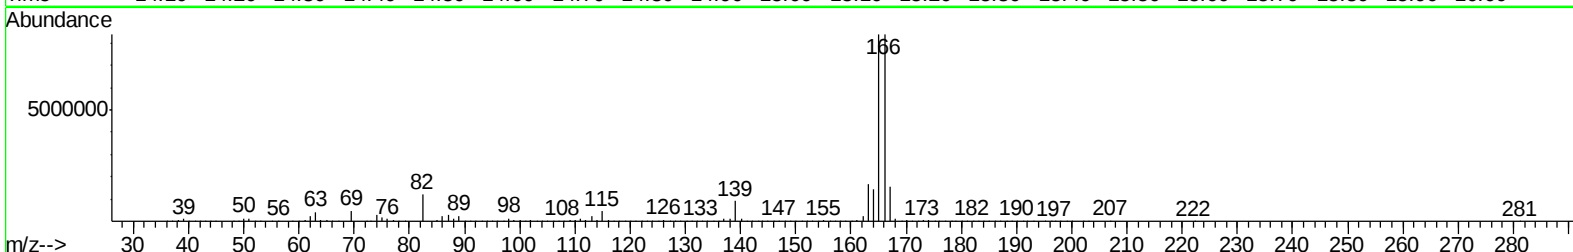


Data File : BM025020.D
Acq On : 22 Feb 2020 11:08
Operator : CG/JU
Sample : L1507-17
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Feb 24 07:01:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 05:59:54 2020
Response via : Initial Calibration

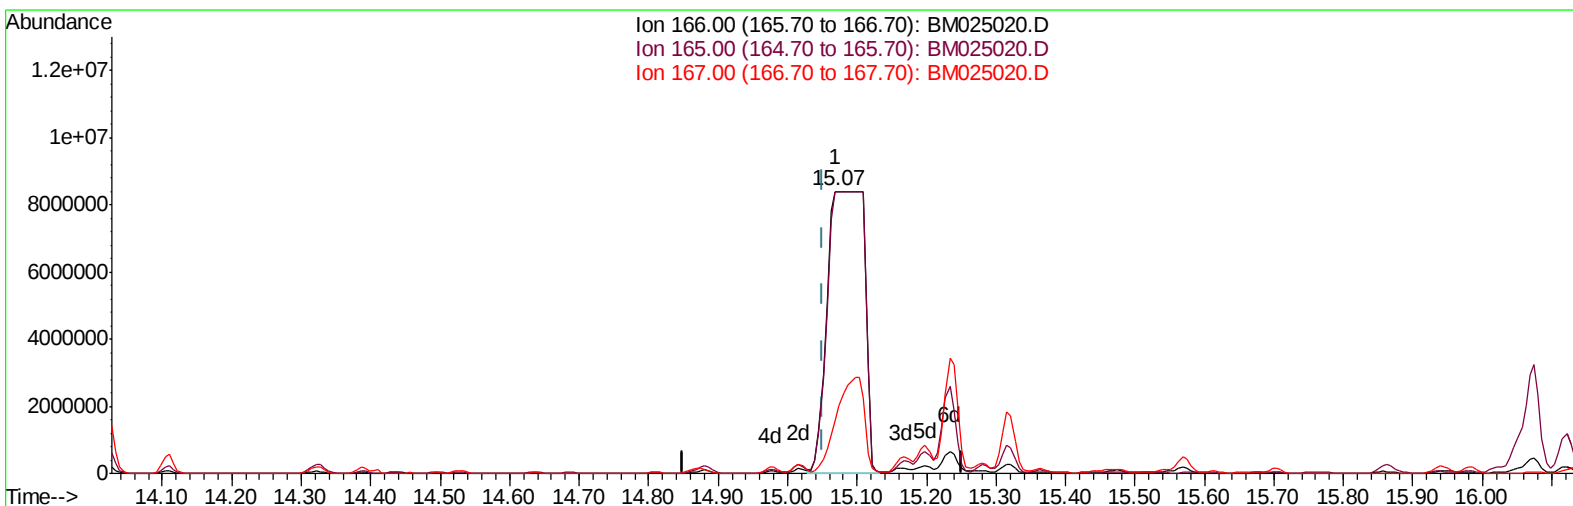

TIC: BM025020.D

(59) Fluorene

15.069min (+0.018) 514.29ng/ul m

response 31147161

Ion	Exp%	Act%
166.00	100	100
165.00	94.80	100.00
167.00	13.30	18.73#
0.00	0.00	0.00