
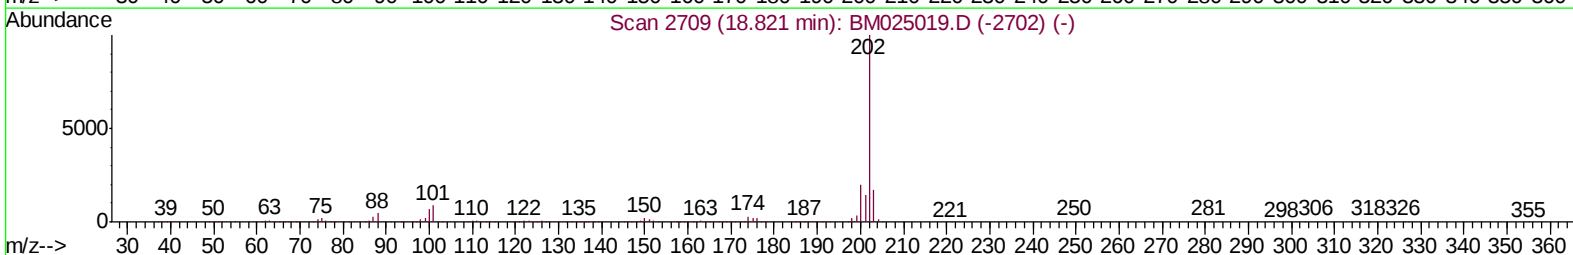
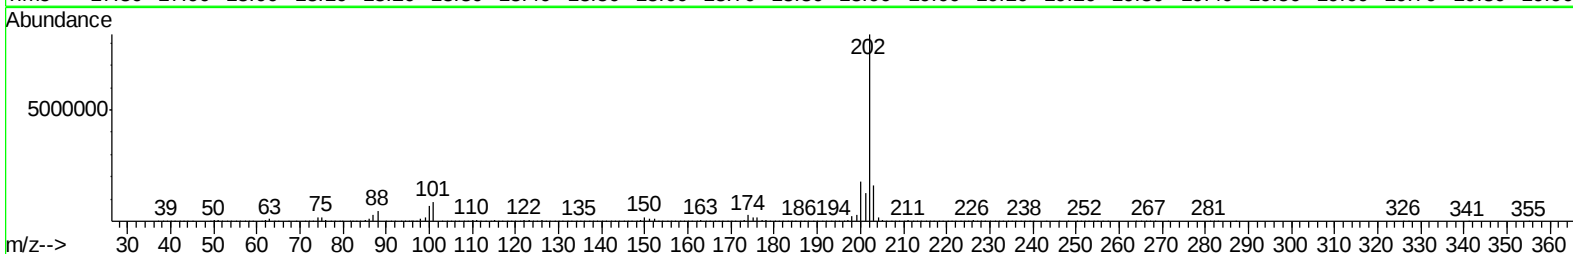


Data File : BM025020.D
Acq On : 22 Feb 2020 11:08
Operator : CG/JU
Sample : L1507-17
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Feb 24 07:01:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 05:59:54 2020
Response via : Initial Calibration

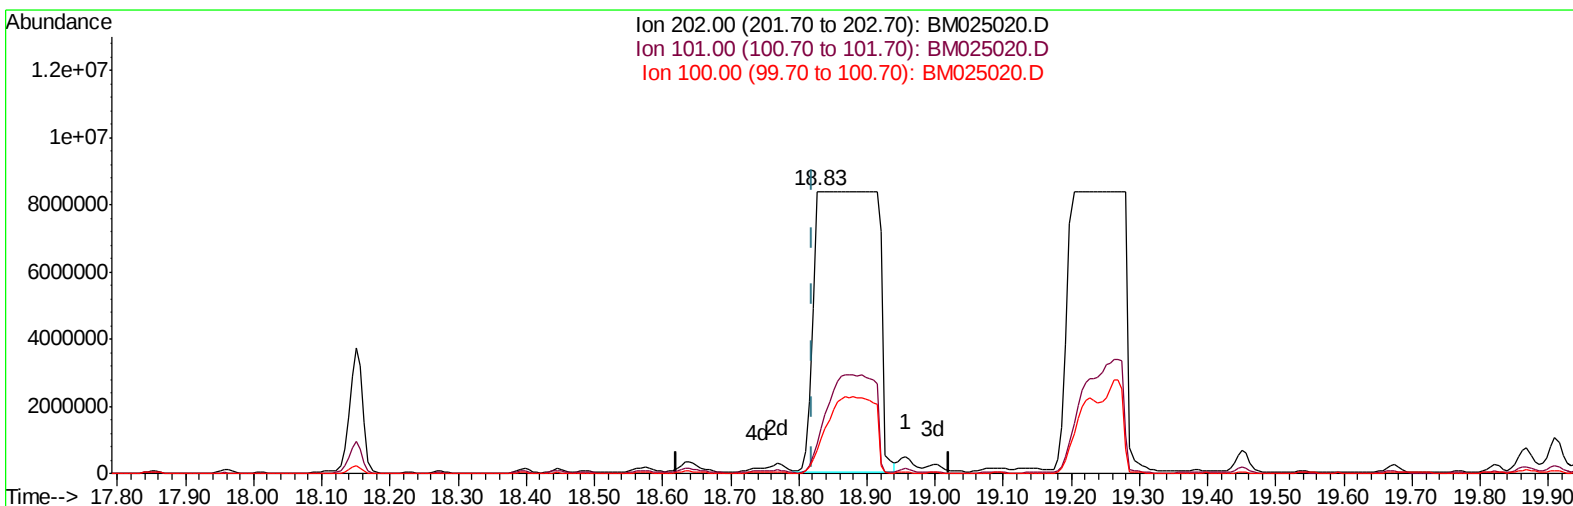

TIC: BM025020.D

(77) Fluoranthene (C)

18.827min (+0.006) 583.35ng/ul m

response 52912612

Ion	Exp%	Act%
202.00	100	100
101.00	7.60	10.42#
100.00	6.00	8.03#
0.00	0.00	0.00