
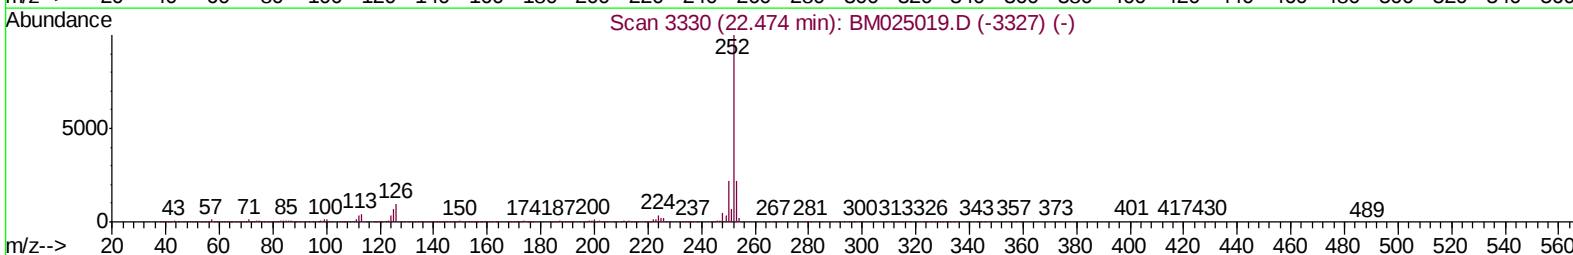
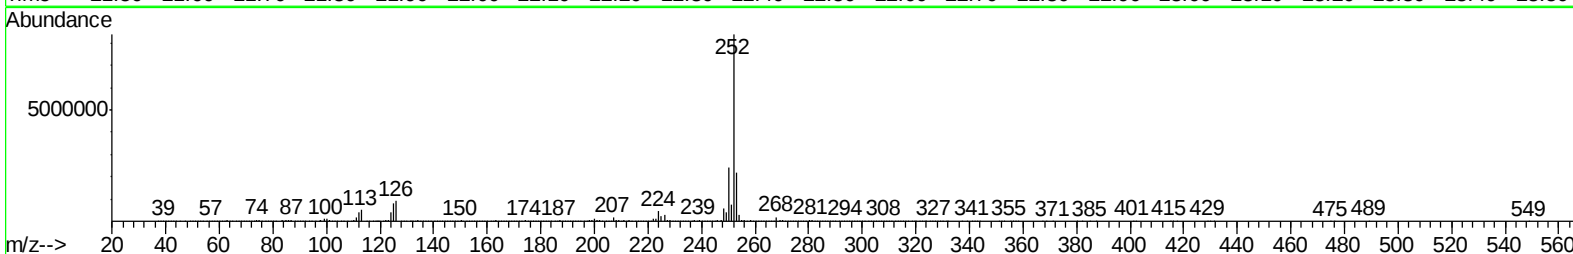


Data File : BM025020.D
Acq On : 22 Feb 2020 11:08
Operator : CG/JU
Sample : L1507-17
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Feb 24 07:01:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 05:59:54 2020
Response via : Initial Calibration

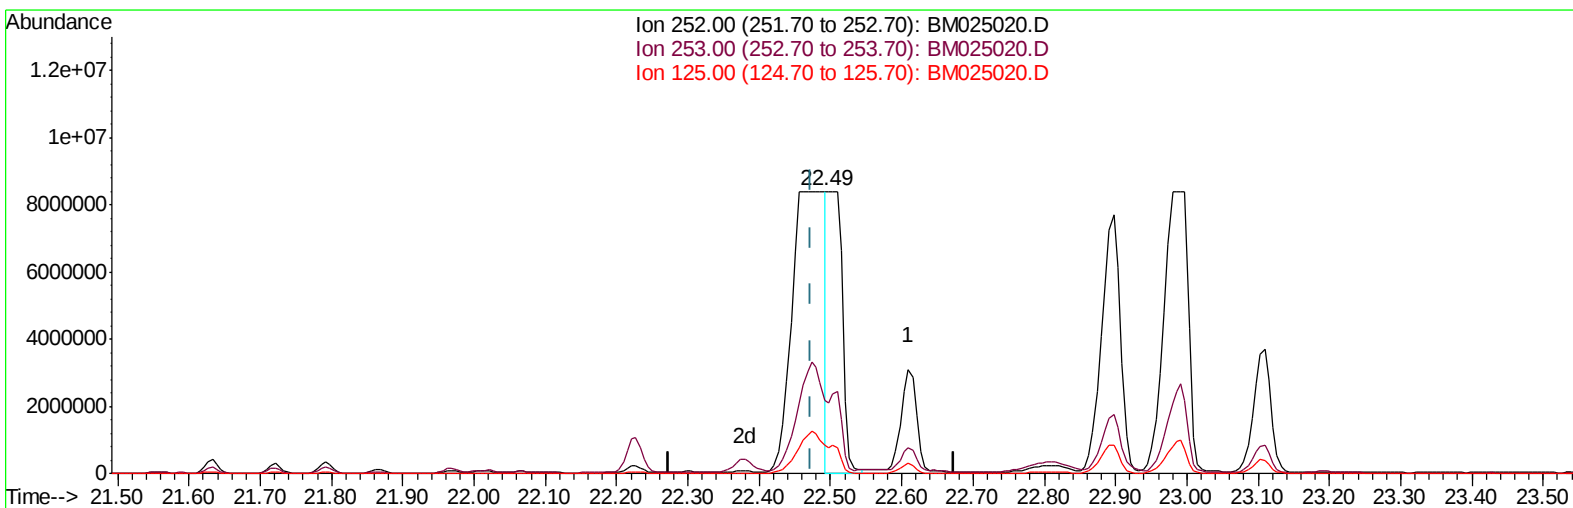

TIC: BM025020.D

(89) Benzo(k)fluoranthene

22.492min (+0.018) 107.59ng/ul m

response 12273693

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	26.05#
125.00	6.40	9.83#
0.00	0.00	0.00