
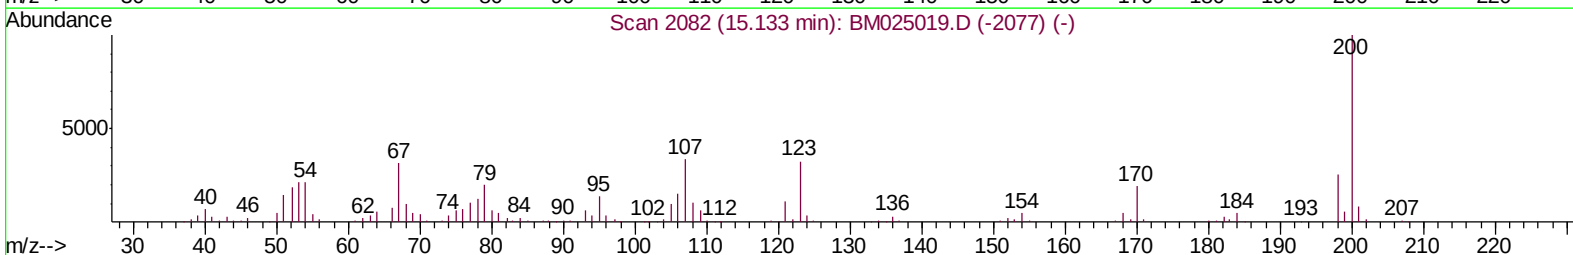
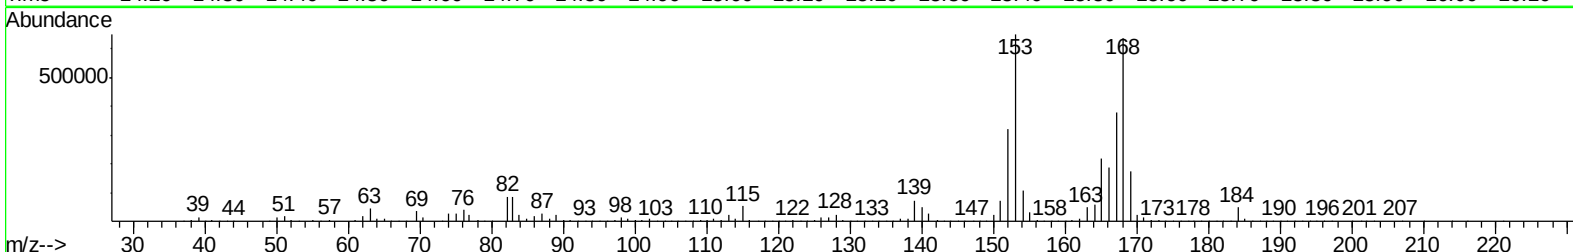


Data File : BM025023.D
Acq On : 22 Feb 2020 12:56
Operator : CG/JU
Sample : L1507-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Feb 24 06:02:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 05:59:54 2020
Response via : Initial Calibration

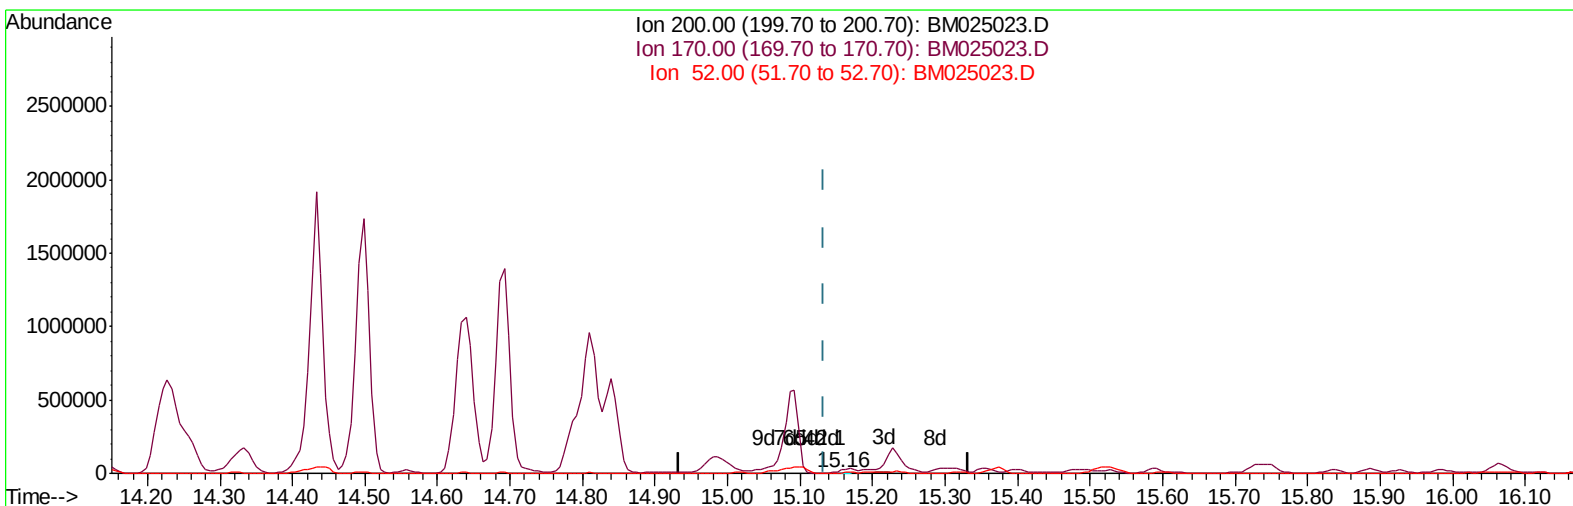

TIC: BM025023.D

(63) 4,6-Dinitro-2-methylphenol-d2 (S)

15.157min (+0.024) 0.03ng/ul

response 283

Ion	Exp%	Act%
200.00	100	100
170.00	18.90	2497.60#
52.00	26.80	446.30#
0.00	0.00	0.00