
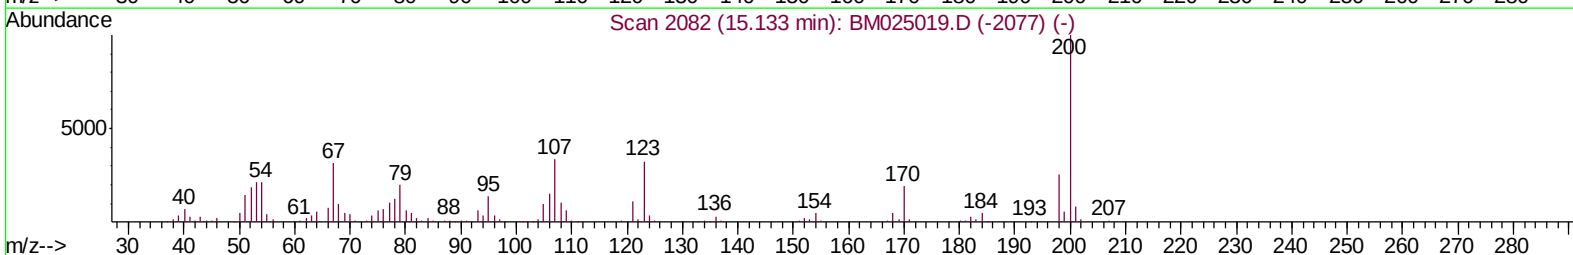
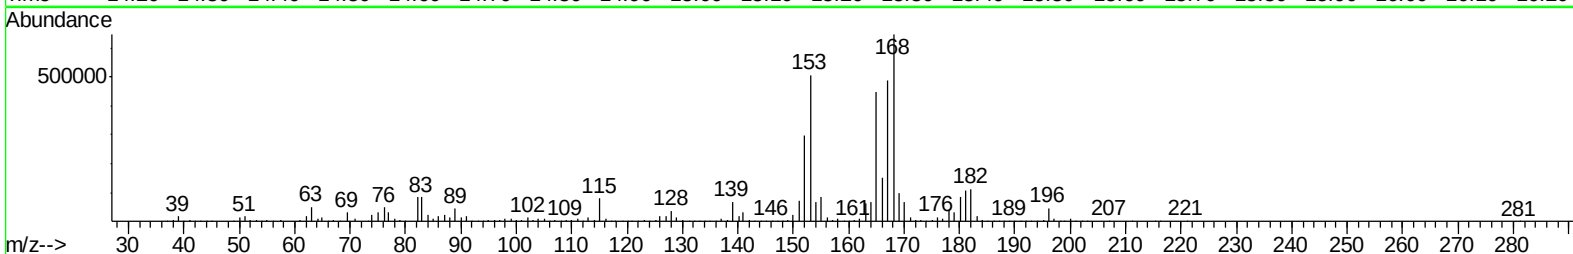


Data File : BM025023.D  
Acq On : 22 Feb 2020 12:56  
Operator : CG/JU  
Sample : L1507-20  
Misc :  
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Feb 24 06:02:24 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM020620MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Mon Feb 24 05:59:54 2020  
Response via : Initial Calibration

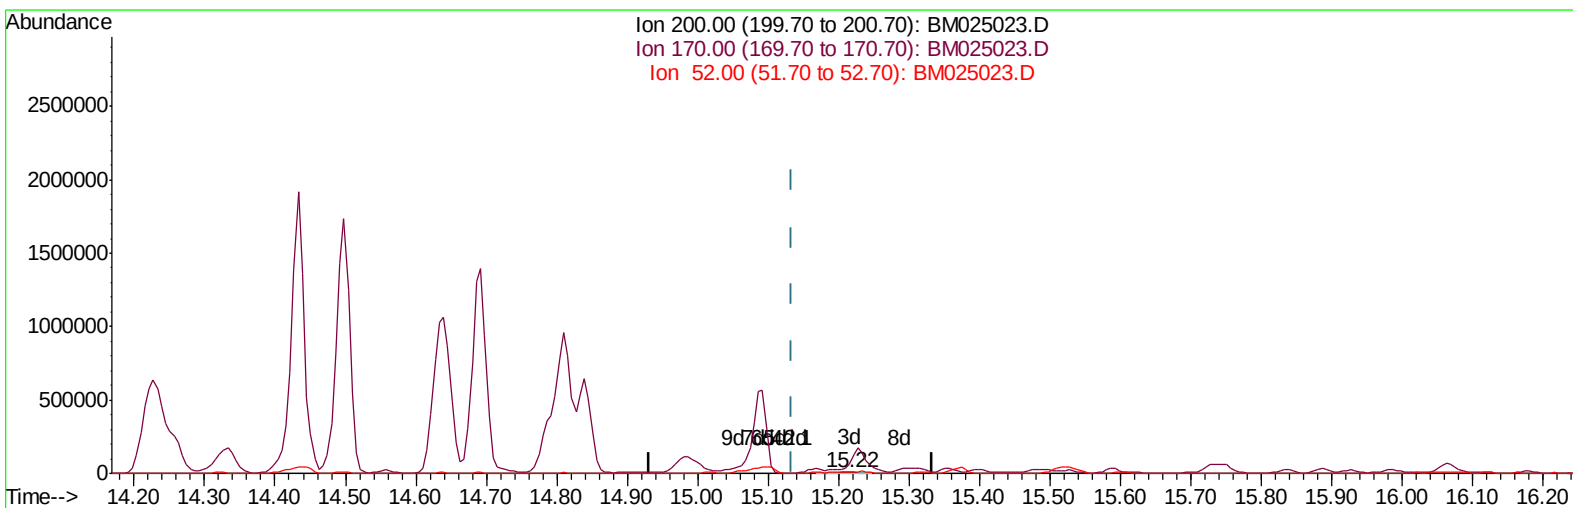

TIC: BM025023.D

(63) 4,6-Dinitro-2-methylphenol-d2 (S)

15.215min (+0.082) 1.50ng/ul m

response 14378

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 200.00 | 100   | 100     |
| 170.00 | 18.90 | 839.22# |
| 52.00  | 26.80 | 64.52#  |
| 0.00   | 0.00  | 0.00    |