
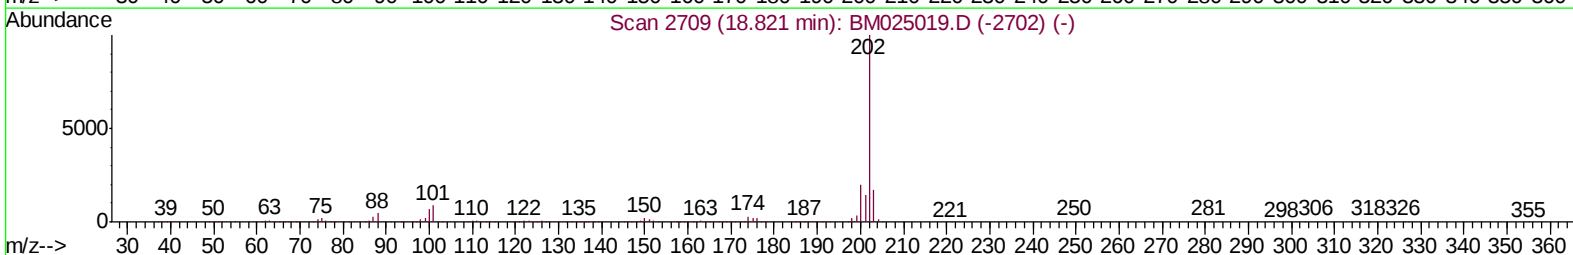
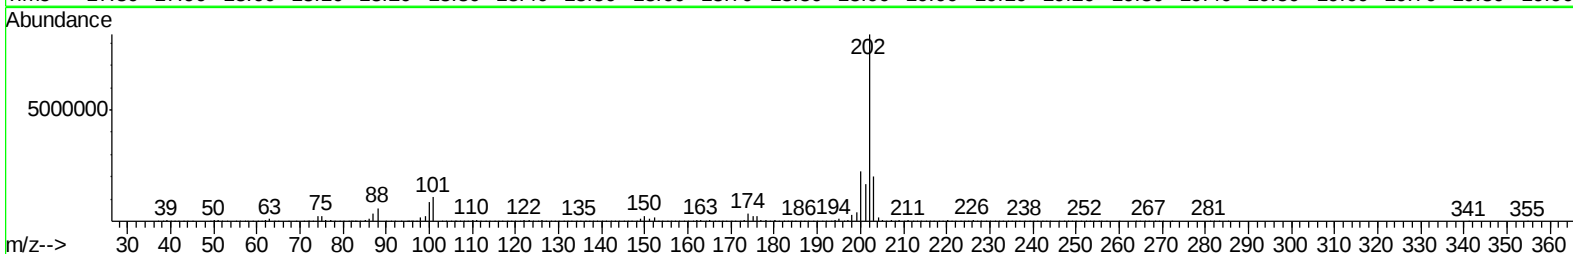


Data File : BM025023.D
Acq On : 22 Feb 2020 12:56
Operator : CG/JU
Sample : L1507-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Feb 24 06:02:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 05:59:54 2020
Response via : Initial Calibration

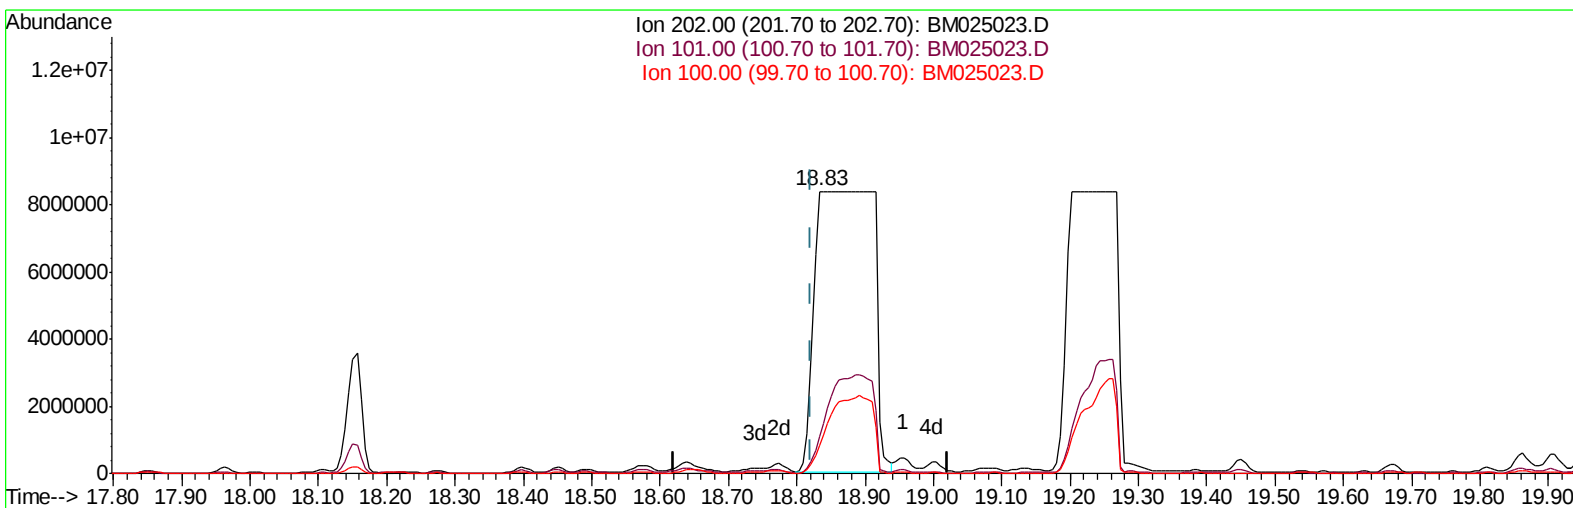

TIC: BM025023.D

(77) Fluoranthene (C)

18.833min (+0.012) 497.41ng/ul m

response 49107394

Ion	Exp%	Act%
202.00	100	100
101.00	7.60	13.01#
100.00	6.00	10.08#
0.00	0.00	0.00