
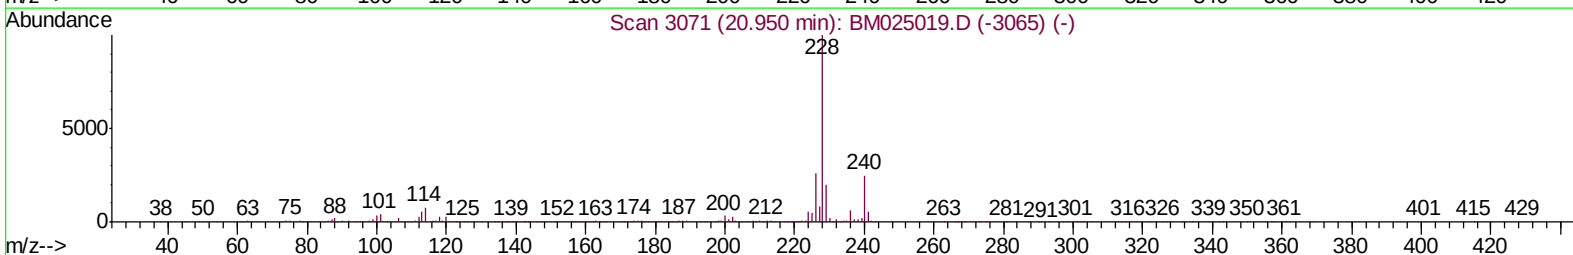
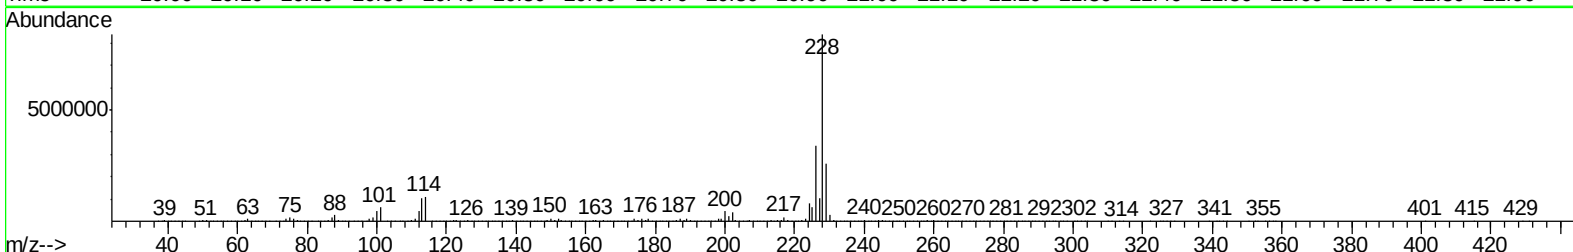


Data File : BM025023.D
Acq On : 22 Feb 2020 12:56
Operator : CG/JU
Sample : L1507-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Feb 24 06:50:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 05:59:54 2020
Response via : Initial Calibration

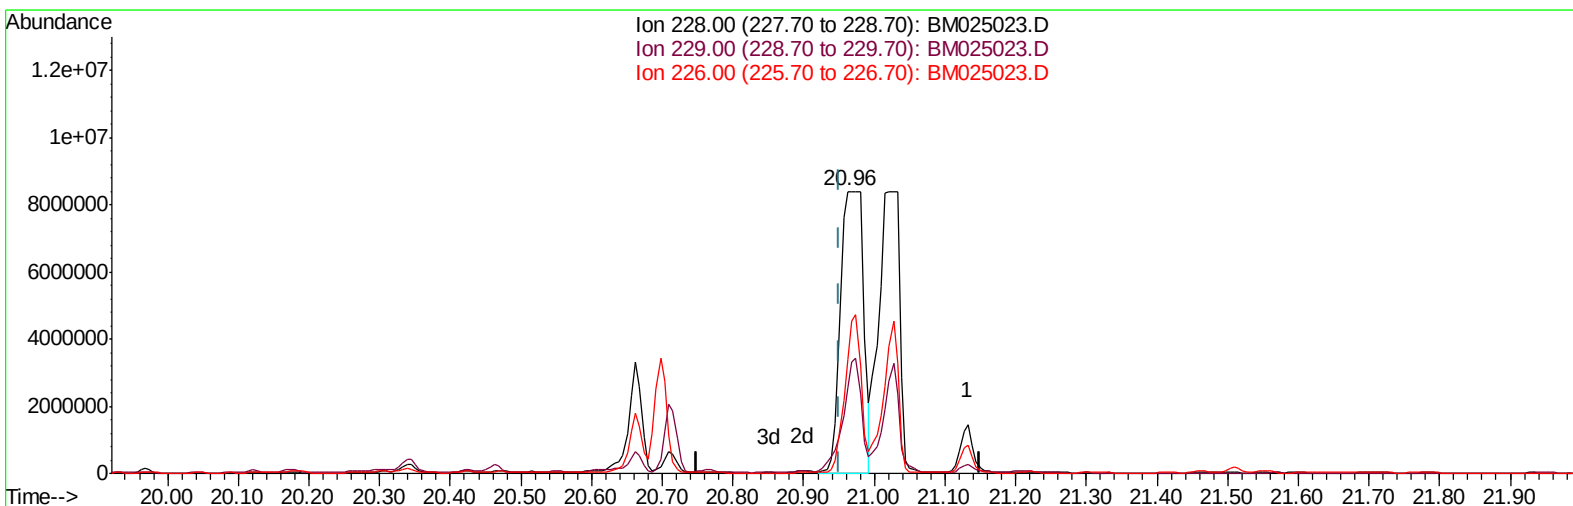

TIC: BM025023.D

(83) Benzo(a)anthracene
20.962min (+0.012) 161.63ng/ul m
response 18850067

Ion	Exp%	Act%
228.00	100	100
229.00	19.90	30.64#
226.00	26.00	40.49#
0.00	0.00	0.00