
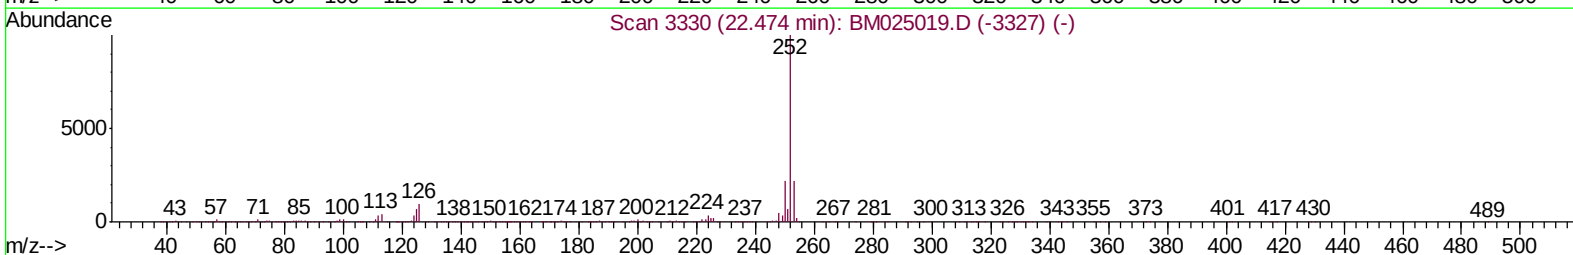
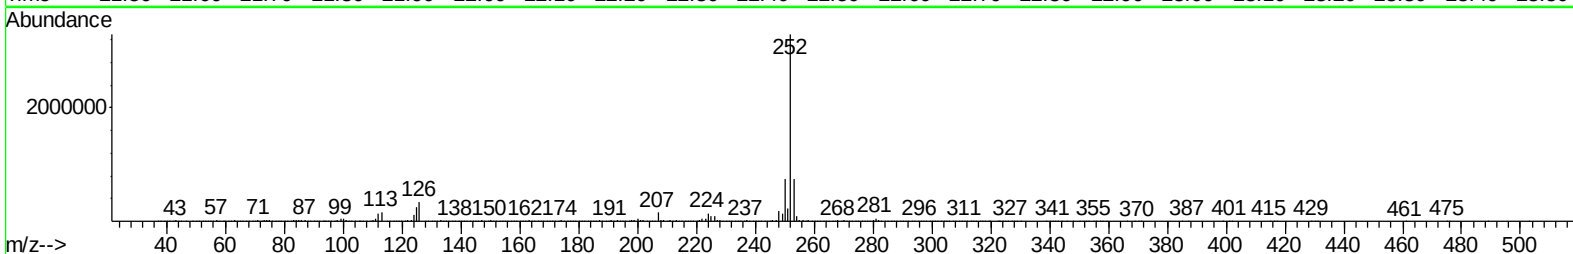


Data File : BM025023.D
Acq On : 22 Feb 2020 12:56
Operator : CG/JU
Sample : L1507-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Feb 24 06:50:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 05:59:54 2020
Response via : Initial Calibration

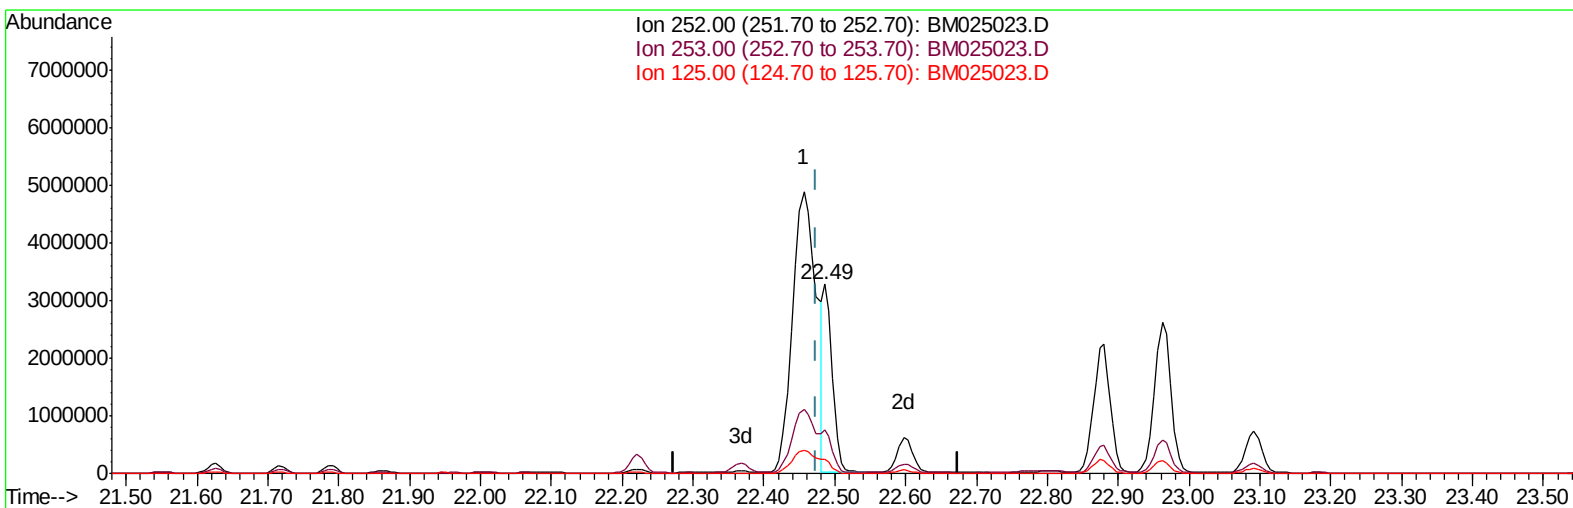

TIC: BM025023.D

(89) Benzo(k)fluoranthene

22.486min (+0.012) 25.86ng/ul m

response 3054807

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	22.69
125.00	6.40	7.64
0.00	0.00	0.00