
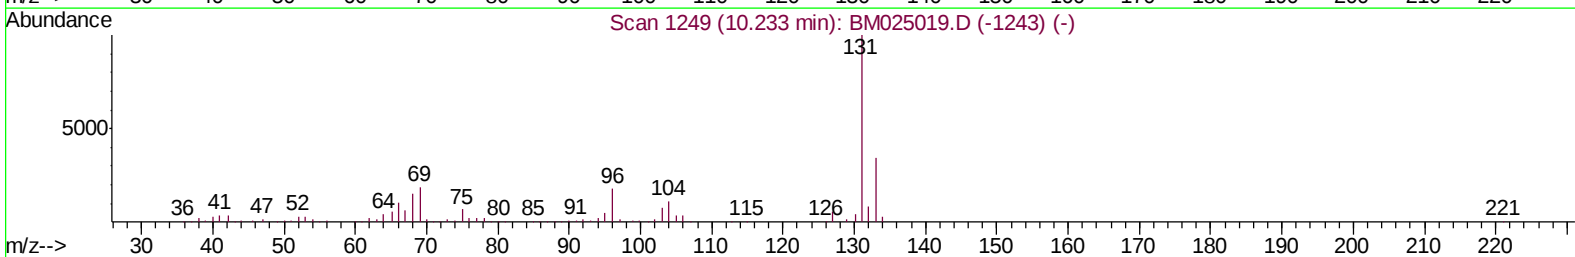
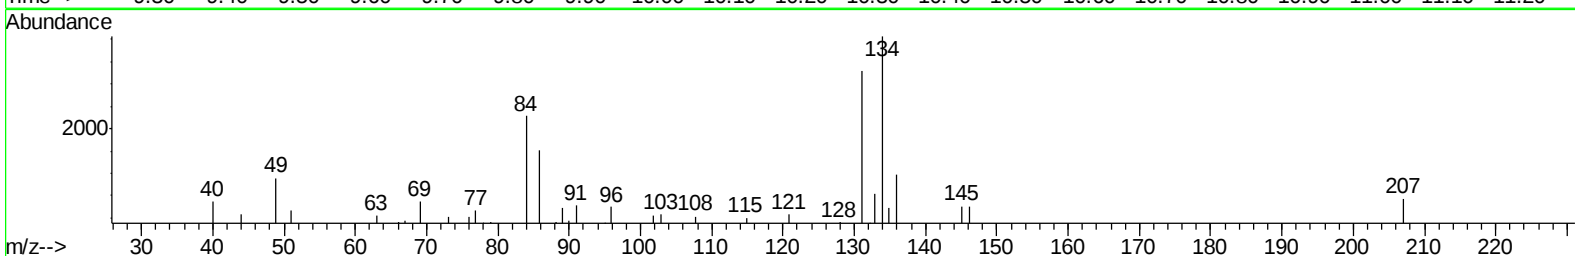


Data File : BM025025.D
Acq On : 22 Feb 2020 14:08
Operator : CG/JU
Sample : L1507-22
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Feb 24 06:02:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 05:59:54 2020
Response via : Initial Calibration

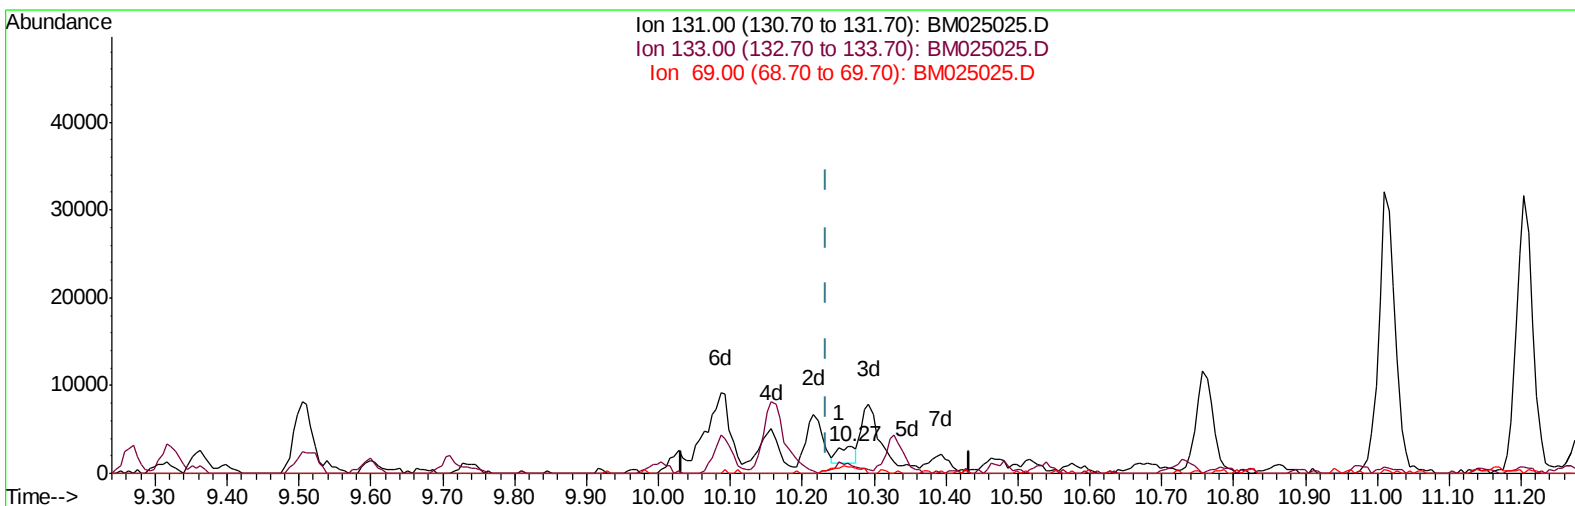

TIC: BM025025.D

(29) 4-Chloroaniline-d4 (S)

10.269min (+0.036) 0.23ng/ul m

response 3473

Ion	Exp%	Act%
131.00	100	100
133.00	34.60	27.50#
69.00	16.20	22.79#
0.00	0.00	0.00