
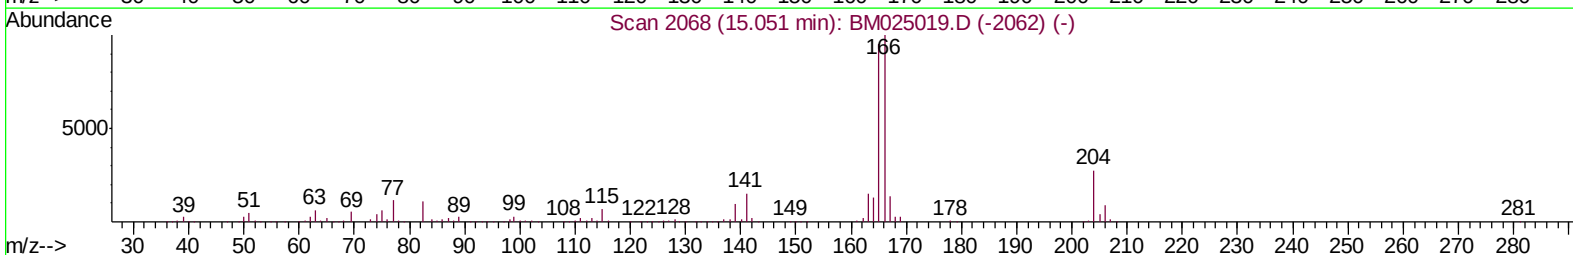
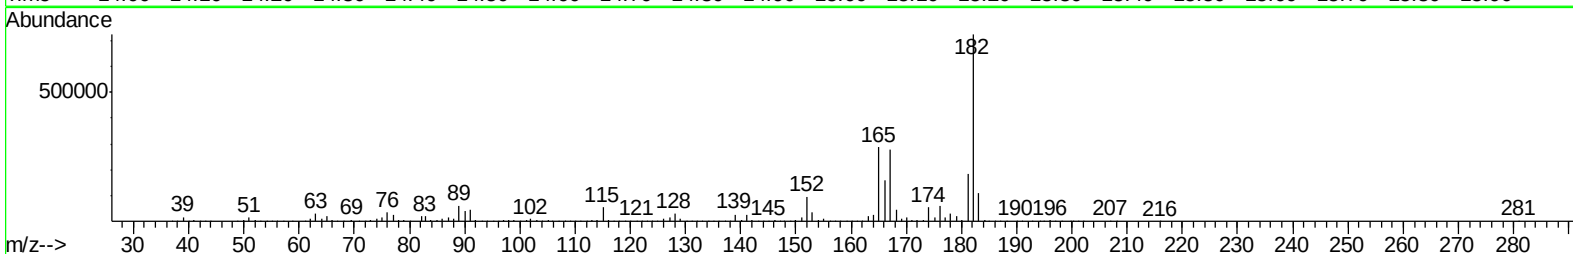


Data File : BM025025.D
Acq On : 22 Feb 2020 14:08
Operator : CG/JU
Sample : L1507-22
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Feb 24 06:02:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 05:59:54 2020
Response via : Initial Calibration

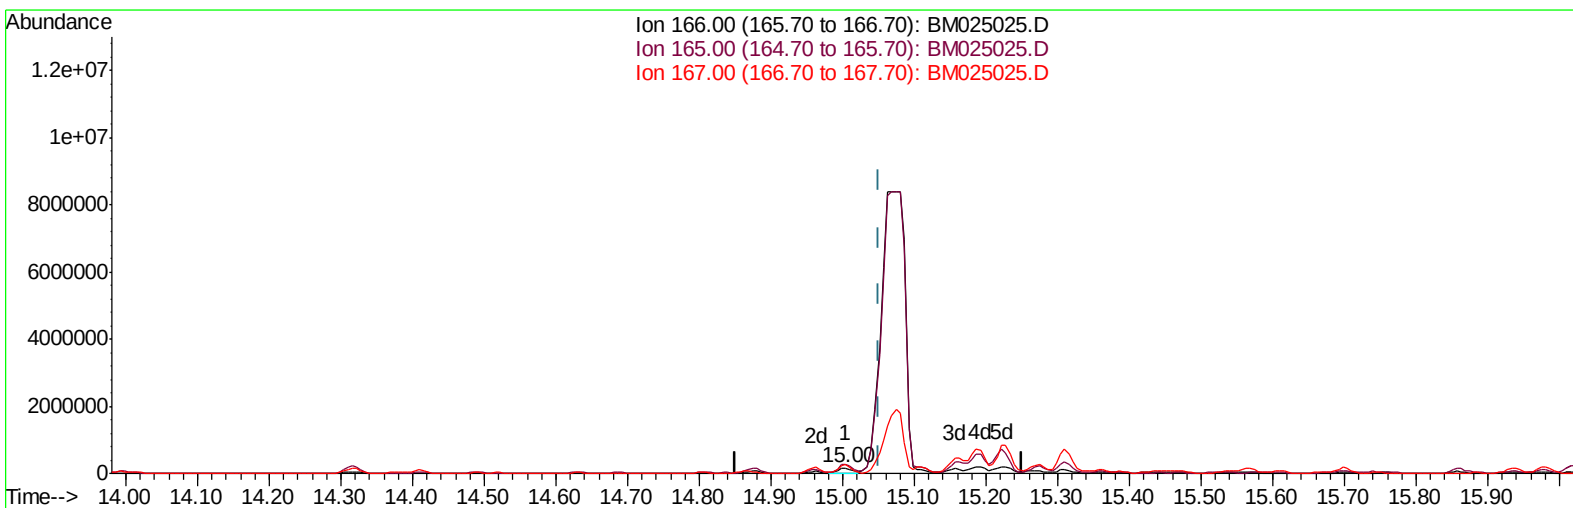

TIC: BM025025.D

(59) Fluorene

15.004min (-0.047) 3.95ng/ul

response 199800

Ion	Exp%	Act%
166.00	100	100
165.00	94.80	181.12#
167.00	13.30	175.86#
0.00	0.00	0.00