
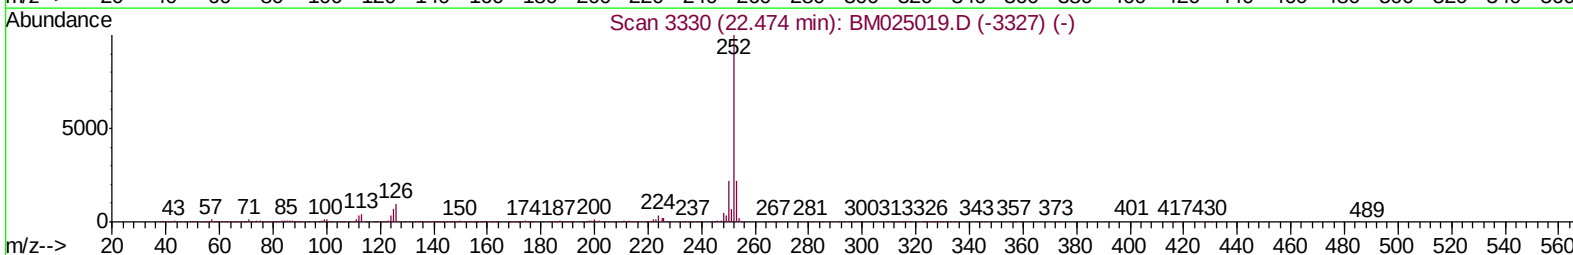
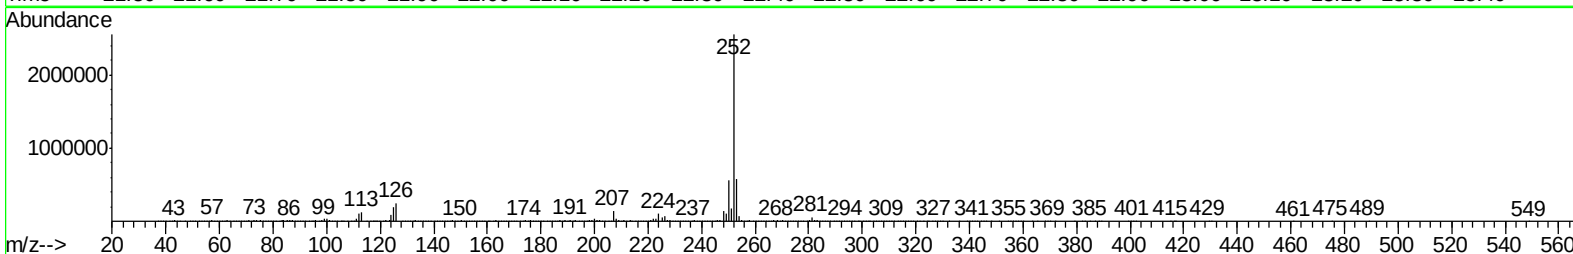


Data File : BM025025.D
Acq On : 22 Feb 2020 14:08
Operator : CG/JU
Sample : L1507-22
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Feb 24 06:02:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 05:59:54 2020
Response via : Initial Calibration

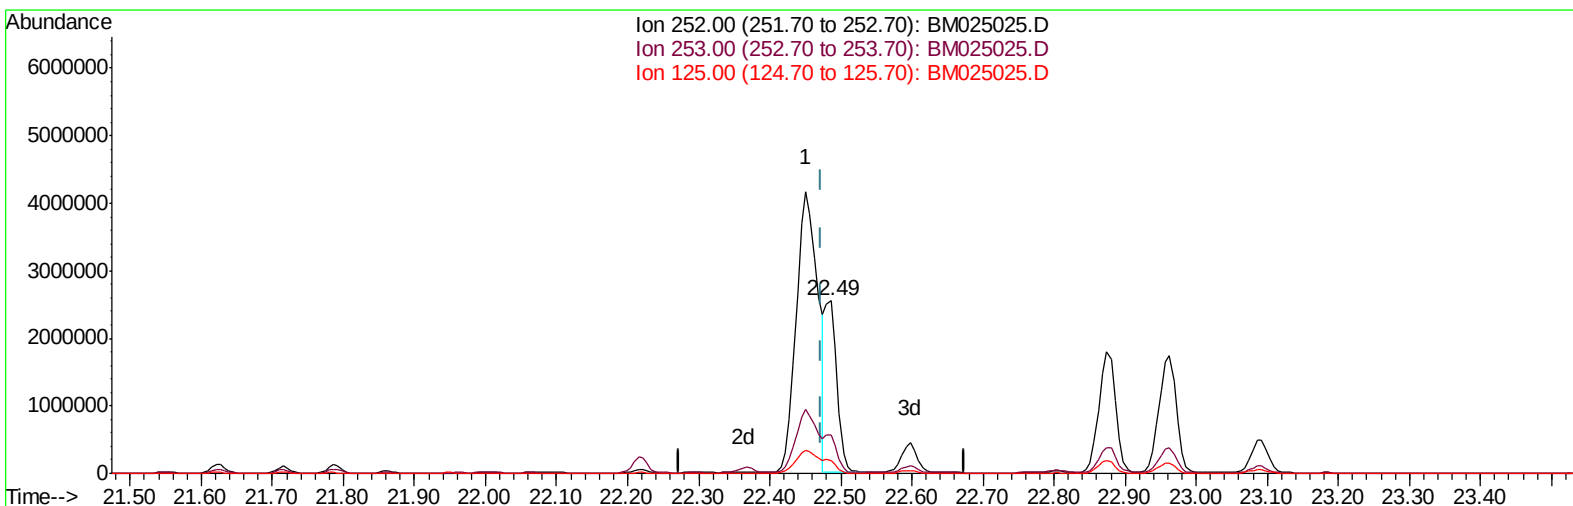

TIC: BM025025.D

(89) Benzo(k)fluoranthene

22.486min (+0.012) 25.31ng/ul m

response 2901671

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	22.36
125.00	6.40	7.34
0.00	0.00	0.00