

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022120\
 Data File : BM025002.D
 Acq On : 22 Feb 2020 00:22
 Operator : CG/JU
 Sample : L1507-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBD02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.557	112	114	121	rVB6	8950	10748	0.42%	0.079%
2	3.699	135	138	139	rBV3	2718	2943	0.11%	0.022%
3	4.404	256	258	261	rBV3	2370	3561	0.14%	0.026%
4	4.528	274	279	289	rVB	20141	32960	1.28%	0.243%
5	4.851	332	334	337	rVV3	2898	2888	0.11%	0.021%
6	5.022	361	363	366	rVB3	3031	3604	0.14%	0.027%
7	5.422	429	431	436	rVB5	2509	2619	0.10%	0.019%
8	5.957	518	522	525	rBV3	2356	3528	0.14%	0.026%
9	6.228	565	568	572	rVB4	2342	3405	0.13%	0.025%
10	6.392	594	596	598	rBV3	2694	2590	0.10%	0.019%
11	6.545	617	622	635	rBV	31660	83283	3.24%	0.613%
12	6.698	642	648	656	rBV	47238	86674	3.37%	0.638%
13	6.881	673	679	692	rVV2	57284	110259	4.29%	0.812%
14	7.198	730	733	734	rBV3	2717	2606	0.10%	0.019%
15	7.339	751	757	768	rBV	421213	714922	27.81%	5.263%
16	7.645	806	809	812	rBV3	1675	2741	0.11%	0.020%
17	8.075	877	882	891	rVV2	36741	80588	3.13%	0.593%
18	8.175	895	899	906	rVB6	5269	10394	0.40%	0.077%
19	8.422	939	941	944	rVB4	2455	2742	0.11%	0.020%
20	8.486	946	952	961	rBV	45573	97969	3.81%	0.721%
21	8.551	961	963	965	rVB3	2907	2572	0.10%	0.019%
22	8.969	1029	1034	1038	rVB3	4199	6432	0.25%	0.047%
23	9.198	1068	1073	1084	rBV	30919	57368	2.23%	0.422%
24	9.751	1160	1167	1176	rBV2	30590	79259	3.08%	0.583%
25	9.828	1178	1180	1184	rVB4	2094	3123	0.12%	0.023%
26	9.904	1191	1193	1197	rVB3	2444	2821	0.11%	0.021%
27	10.092	1217	1225	1238	rBV	581440	991480	38.57%	7.298%
28	10.263	1249	1254	1259	rBV3	18584	42964	1.67%	0.316%
29	10.580	1305	1308	1312	rBV3	1732	2733	0.11%	0.020%
30	11.398	1441	1447	1448	rBV4	2241	3191	0.12%	0.023%
31	12.921	1700	1706	1713	rBV3	12540	22241	0.87%	0.164%
32	13.327	1773	1775	1779	rBV2	2162	3442	0.13%	0.025%
33	13.427	1785	1792	1798	rBV	147907	249428	9.70%	1.836%
34	13.474	1798	1800	1807	rVB2	19169	27871	1.08%	0.205%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022120\
 Data File : BM025002.D
 Acq On : 22 Feb 2020 00:22
 Operator : CG/JU
 Sample : L1507-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBD02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Title : SVOA CALIBRATION

35	13.680	1829	1835	1846	rBV	185820	290997	11.32%	2.142%
36	13.992	1882	1888	1898	rBV	910603	1383817	53.83%	10.186%
37	15.004	2054	2060	2072	rBV	246369	416491	16.20%	3.066%
38	15.151	2081	2085	2096	rVB3	13716	25717	1.00%	0.189%
39	16.751	2350	2357	2369	rBV	1134897	1677747	65.26%	12.350%
40	16.851	2369	2374	2391	rVB	249095	445257	17.32%	3.278%
41	17.186	2426	2431	2435	rBV5	6250	9997	0.39%	0.074%
42	17.368	2456	2462	2465	rBV6	2593	5301	0.21%	0.039%
43	17.621	2500	2505	2506	rBV5	3167	3902	0.15%	0.029%
44	17.703	2516	2519	2522	rBV5	9641	12694	0.49%	0.093%
45	17.833	2536	2541	2544	rBV6	8179	13503	0.53%	0.099%
46	17.998	2566	2569	2571	rBV4	3536	4949	0.19%	0.036%
47	18.339	2624	2627	2628	rBV2	2900	3664	0.14%	0.027%
48	18.374	2630	2633	2634	rBV2	3042	2884	0.11%	0.021%
49	18.568	2663	2666	2669	rBV3	6593	6707	0.26%	0.049%
50	18.698	2685	2688	2691	rBV4	9192	11380	0.44%	0.084%
51	18.821	2705	2709	2716	rVB	53982	73450	2.86%	0.541%
52	18.927	2724	2727	2728	rBV3	5021	4965	0.19%	0.037%
53	19.156	2760	2766	2770	rBV	455335	701544	27.29%	5.164%
54	19.539	2826	2831	2836	rBV4	12907	27438	1.07%	0.202%
55	19.674	2849	2854	2863	rBV6	25443	69762	2.71%	0.514%
56	19.856	2882	2885	2890	rVB3	19566	22197	0.86%	0.163%
57	19.992	2905	2908	2913	rBV	28459	42412	1.65%	0.312%
58	20.962	3068	3073	3089	rVB	1663984	2429308	94.50%	17.882%
59	22.909	3400	3404	3409	rBV	361375	572261	22.26%	4.212%
60	23.038	3421	3426	3439	rVB	1432829	2570729	100.00%	18.923%


Sum of corrected areas: 13585022

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022120\
Data File : BM025002.D
Acq On : 22 Feb 2020 00:22
Operator : CG/JU
Sample : L1507-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

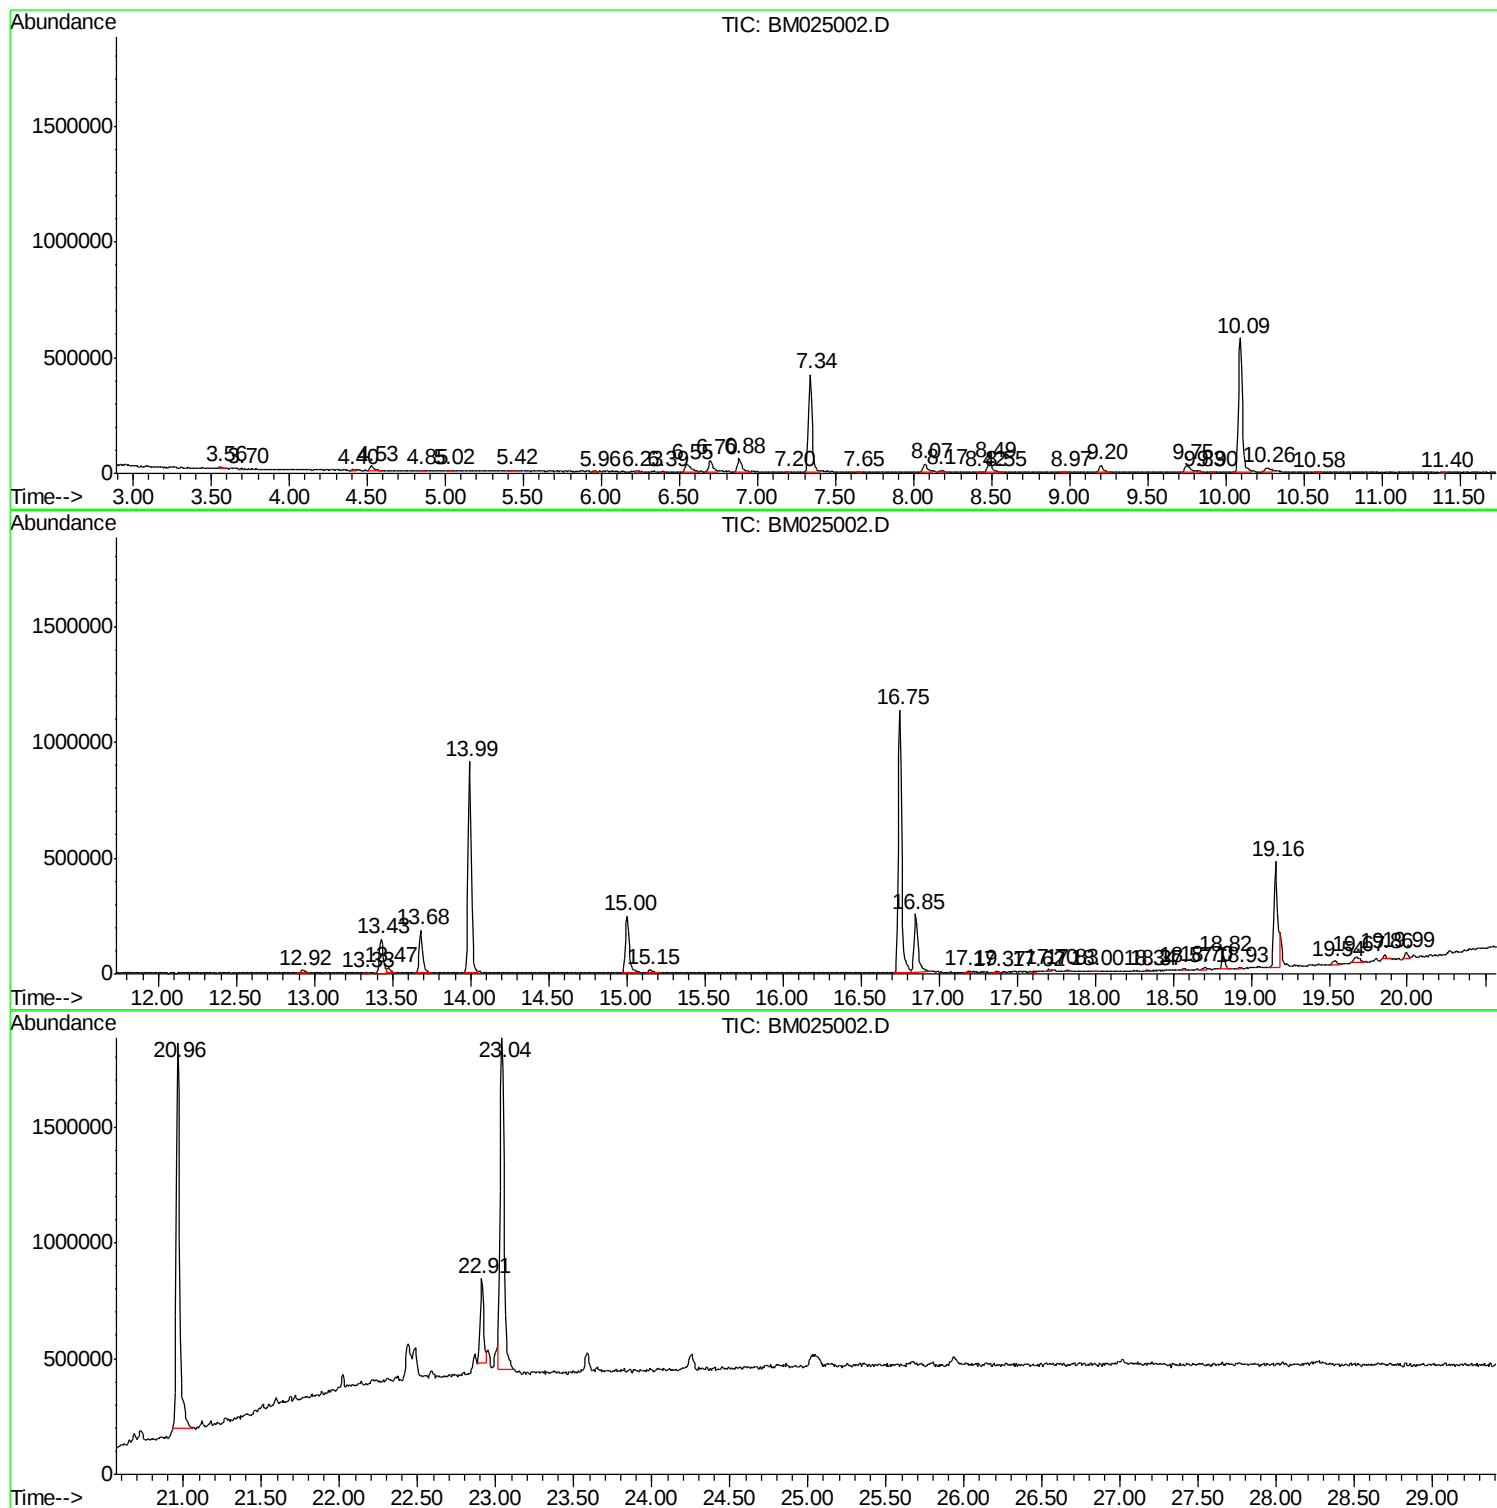

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022120\
Data File : BM025002.D
Acq On : 22 Feb 2020 00:22
Operator : CG/JU
Sample : L1507-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022120\
Data File : BM025002.D
Acq On : 22 Feb 2020 00:22
Operator : CG/JU
Sample : L1507-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc