

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025039.D

Acq On : 25 Feb 2020 12:13

Operator : CG/JU

Sample : PB126806BL

Misc :

ALS Vial : 5 Sample Multiplier: 1

Quant Time: Feb 25 14:01:19 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :


SBLK06

Manual Integrations

APPROVED

mohammad

2/26/2020 6:48:15 AM

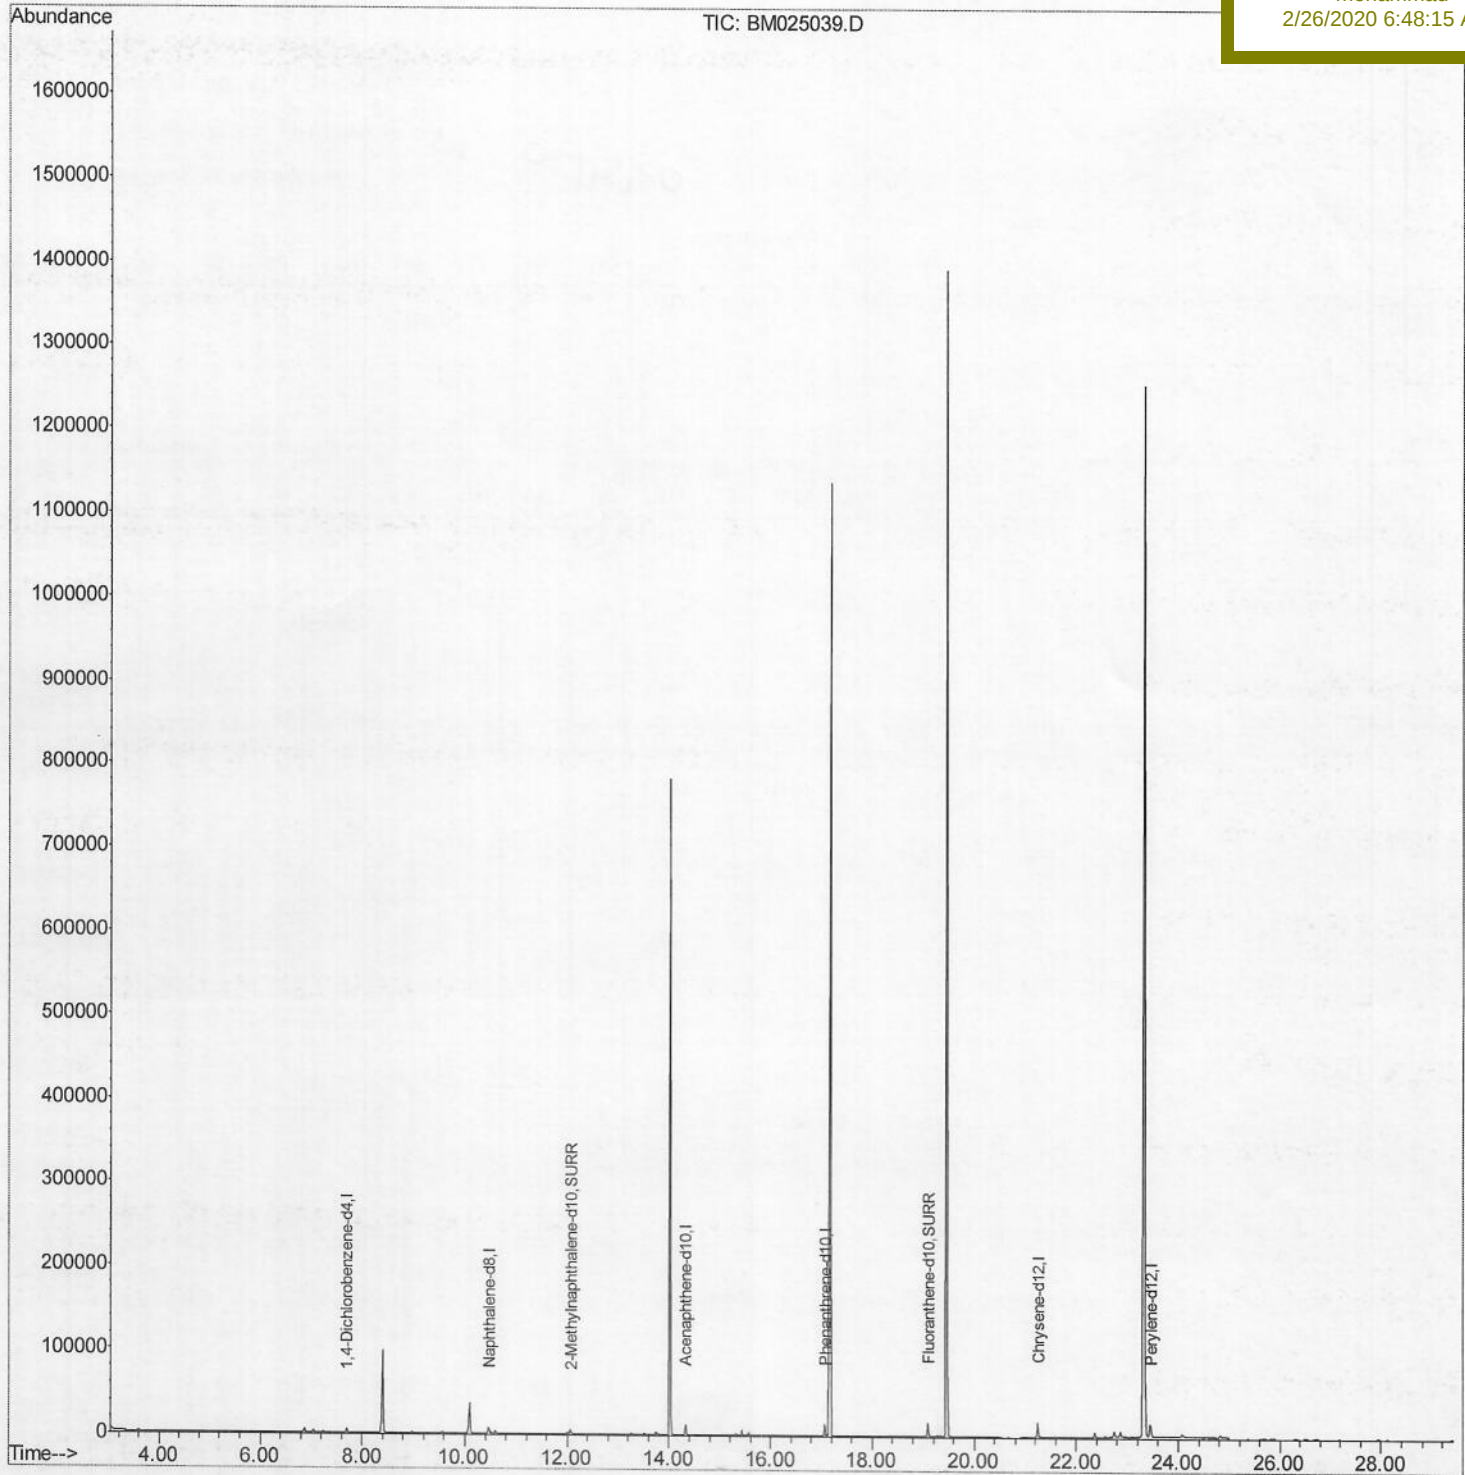

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
 Data File : BM025039.D
 Acq On : 25 Feb 2020 12:13
 Operator : CG/JU
 Sample : PB126806BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Feb 25 13:59:53 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 25 11:03:43 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 SBLK06

Manual Integrations
 APPROVED

mohammad
 2/26/2020 6:48:15 AM

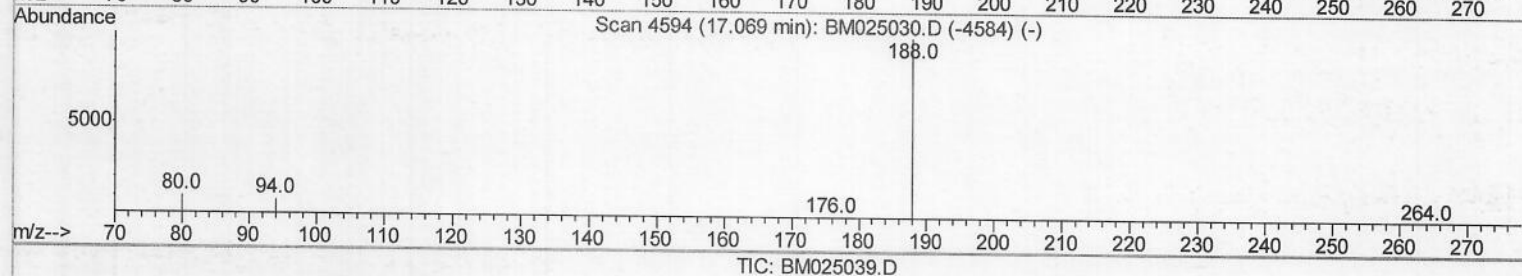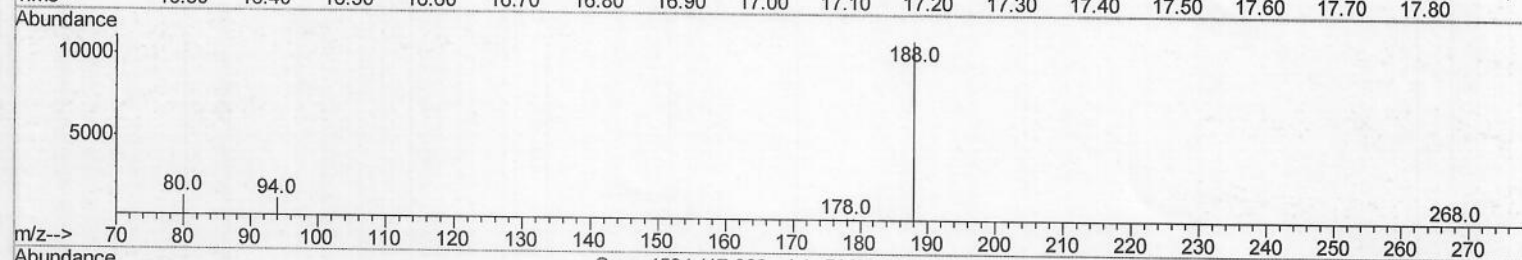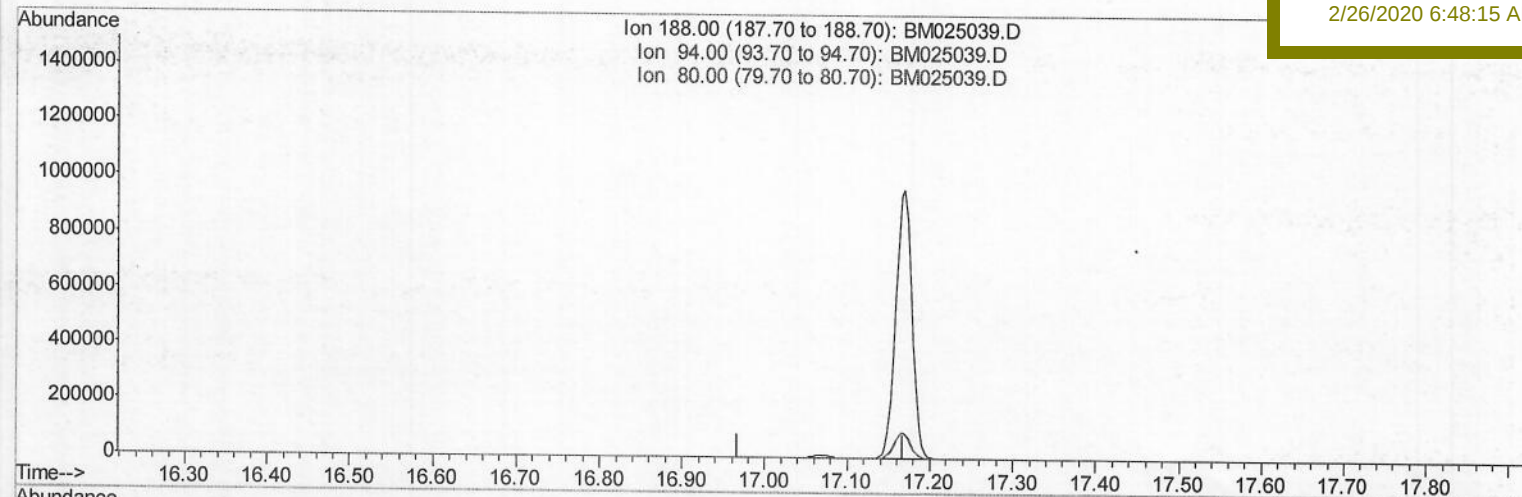

TIC: BM025039.D

(10) Phenanthrene-d10 (I)
 17.068min (-17.068) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025039.D

Acq On : 25 Feb 2020 12:13

Operator : CG/JU

Sample : PB126806BL

Misc :

ALS Vial : 5 Sample Multiplier: 1

Quant Time: Feb 25 13:59:53 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

SBLK06

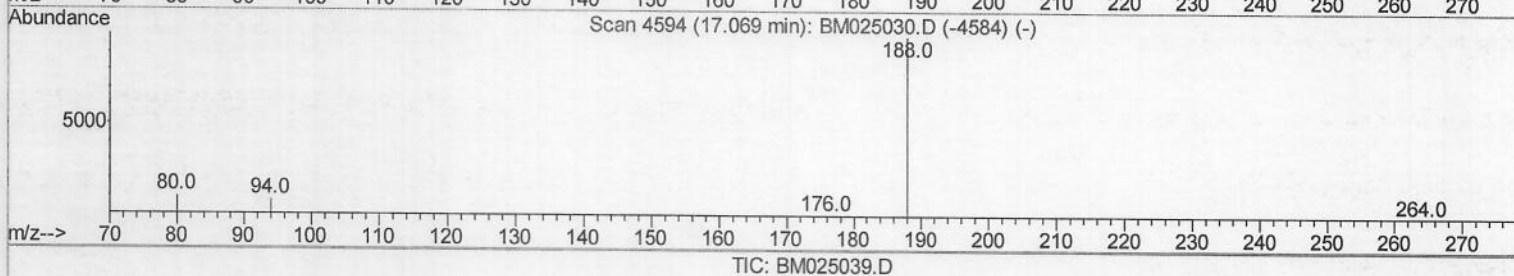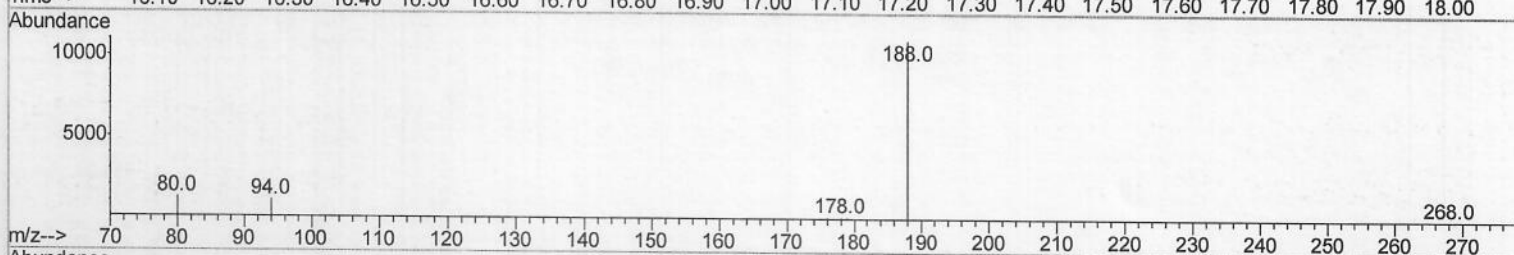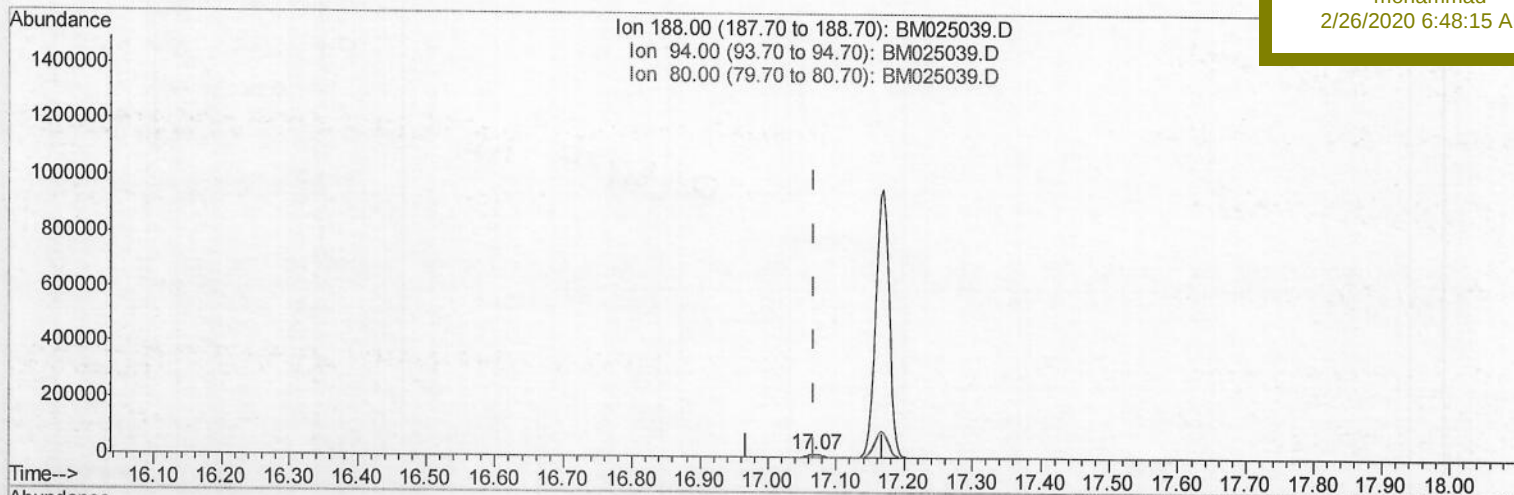Manual Integrations
APPROVEDmohammad
2/26/2020 6:48:15 AM

(10) Phenanthrene-d10 (I)

17.069min (+0.001) 0.40ng/ul m > 86 02/26/20

response 15076

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	9.85#
80.00	22.60	11.10#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
Data File : BM025039.D
Acq On : 25 Feb 2020 12:13
Operator : CG/JU
Sample : PB126806BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
Client Sample Id :
SBLK06

Manual Integrations
APPROVED

mohammad
2/26/2020 6:48:15 AM

Quant Time: Feb 25 14:01:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	2226	0.40	ng/ul	0.00
2) Naphthalene-d8	10.47	136	9288	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.33	164	6463	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.07	188	15076m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	16279	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	17508	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.07	152	6028	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.10	212	17211	0.33	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 02/26/20