

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025041.D

Acq On : 25 Feb 2020 13:25

Operator : CG/JU

Sample : PB126774BL

Misc :

ALS Vial : 7 Sample Multiplier: 1

Quant Time: Feb 25 14:03:38 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :


SBLK74

Manual Integrations

APPROVED

mohammad

2/26/2020 6:48:23 AM

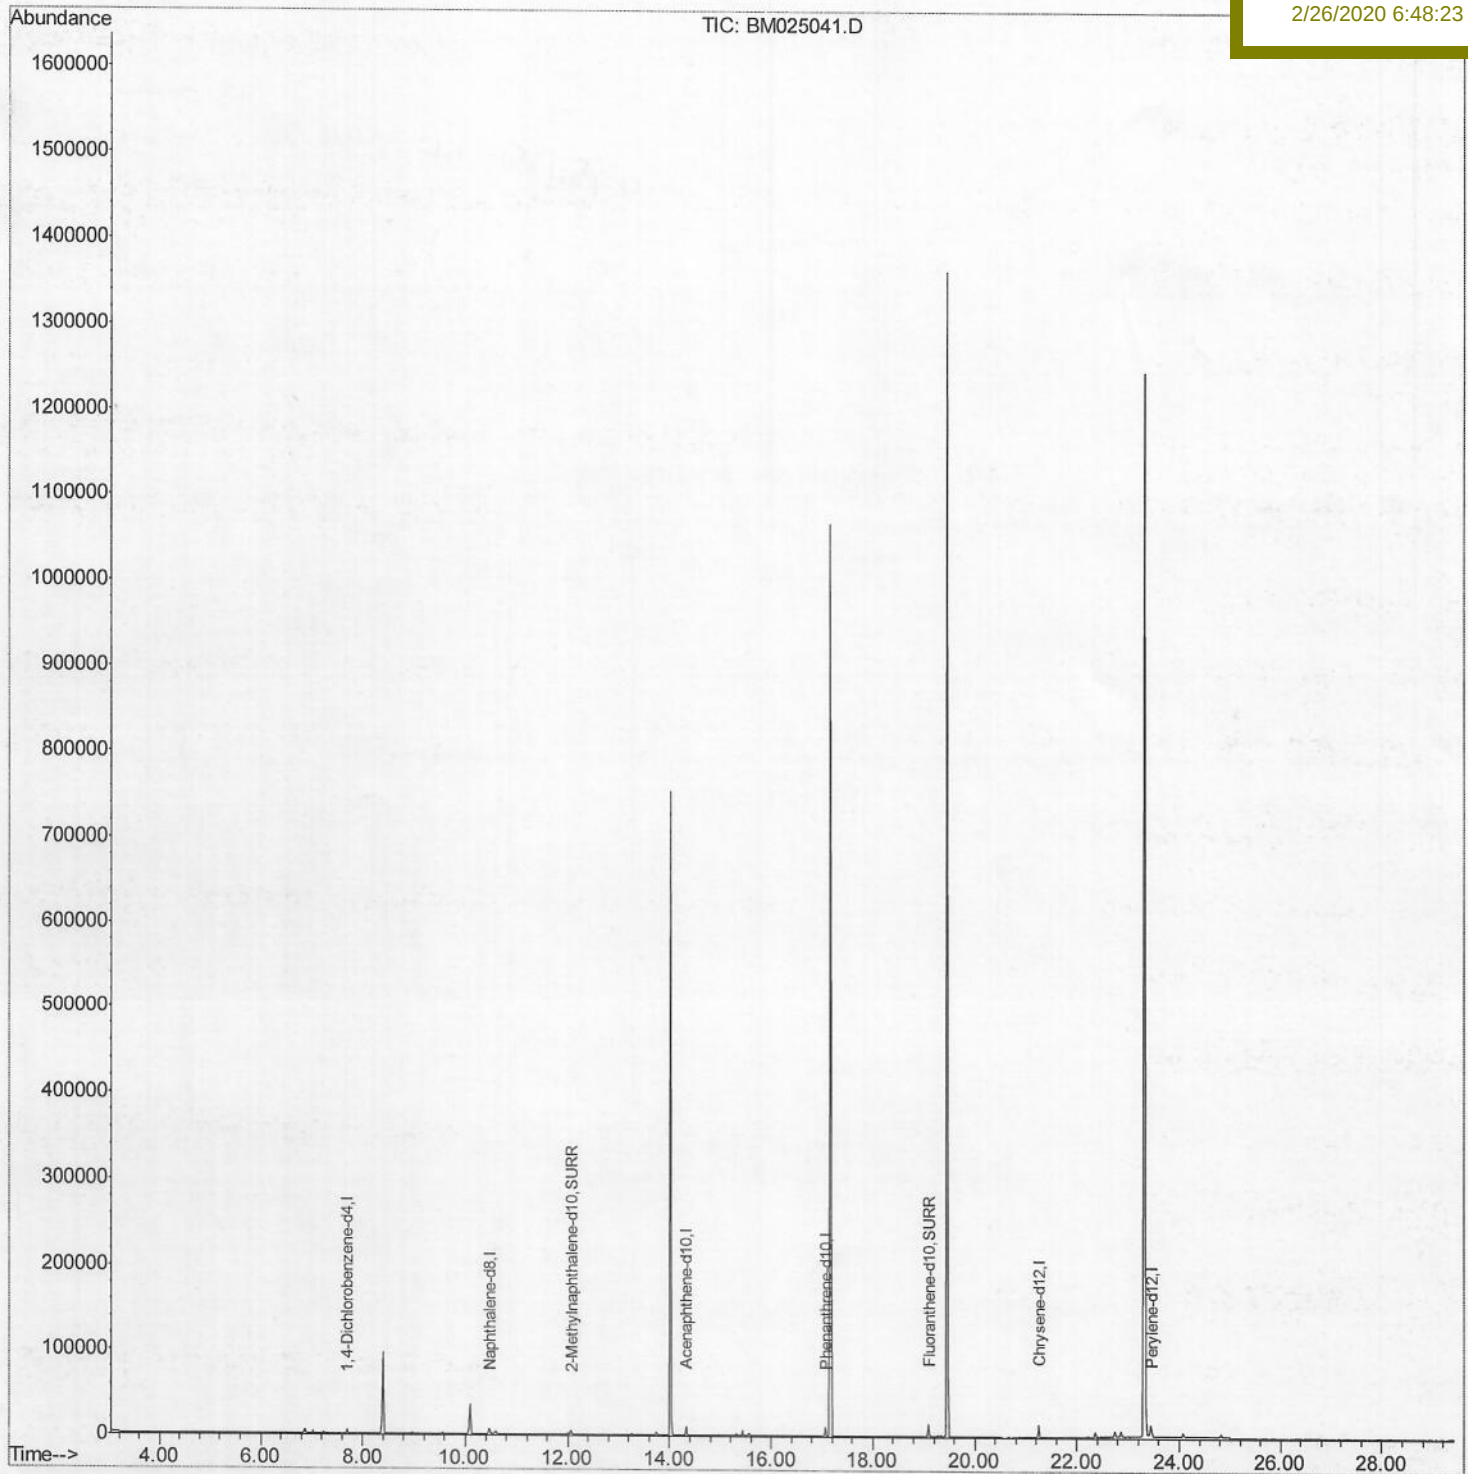

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025041.D

Acq On : 25 Feb 2020 13:25

Operator : CG/JU

Sample : PB126774BL

Misc :

ALS Vial : 7 Sample Multiplier: 1

Quant Time: Feb 25 14:02:51 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




SBLK74

Manual Integrations

APPROVED

mohammad

2/26/2020 6:48:23 AM

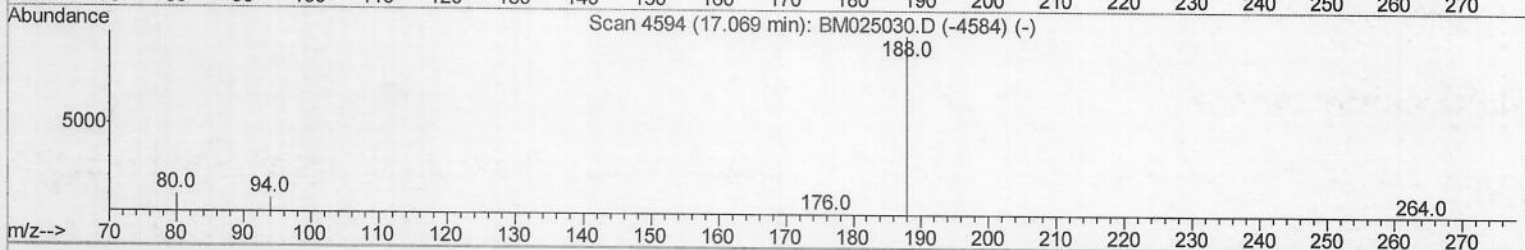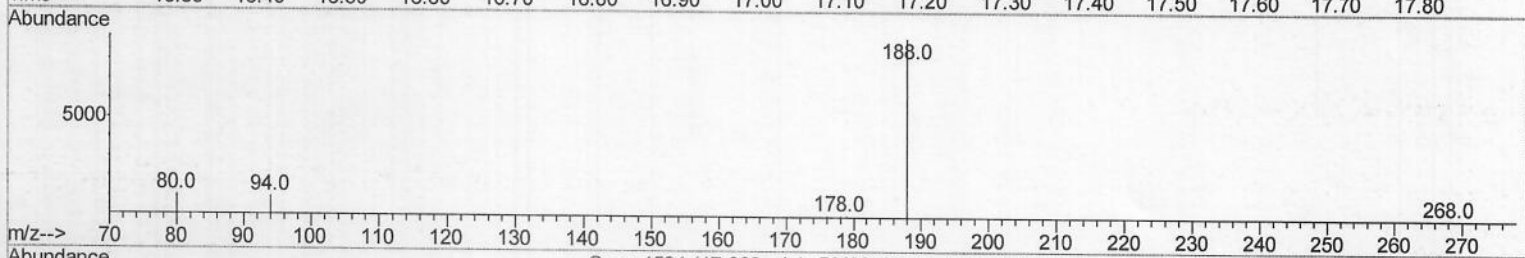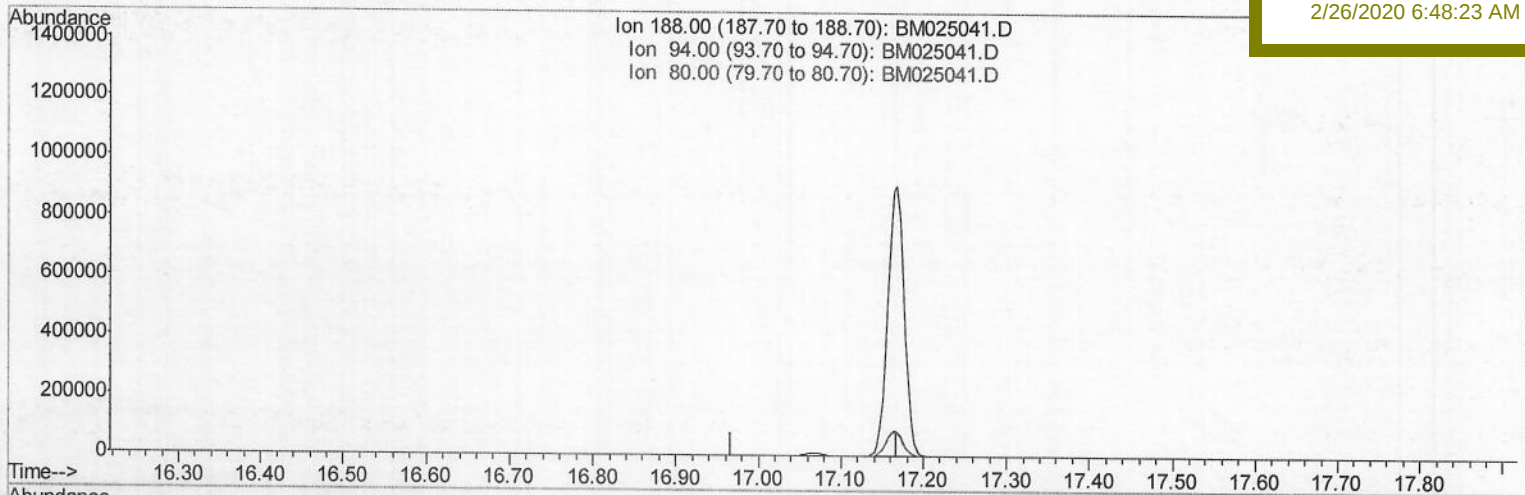

TIC: BM025041.D

(10) Phenanthrene-d10 (I)

17.068min (-17.068) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
Data File : BM025041.D
Acq On : 25 Feb 2020 13:25
Operator : CG/JU
Sample : PB126774BL
Misc :
ALS Vial : 7 Sample Multiplier: 1




Quant Time: Feb 25 14:02:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

SBLK74

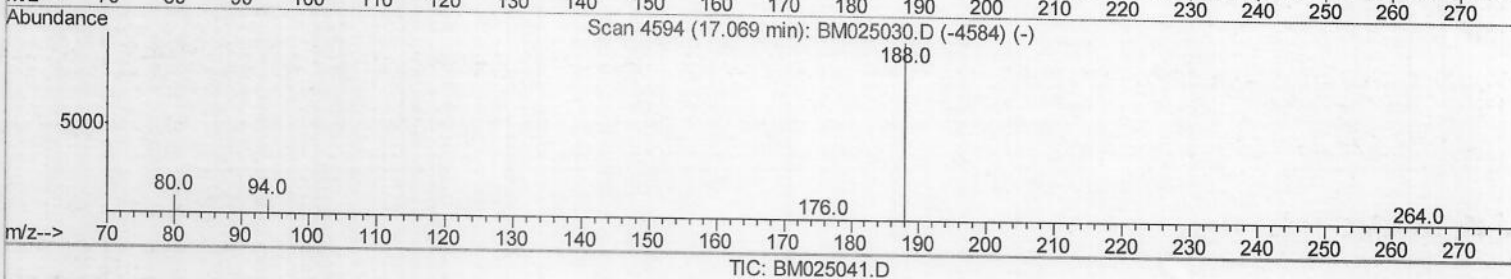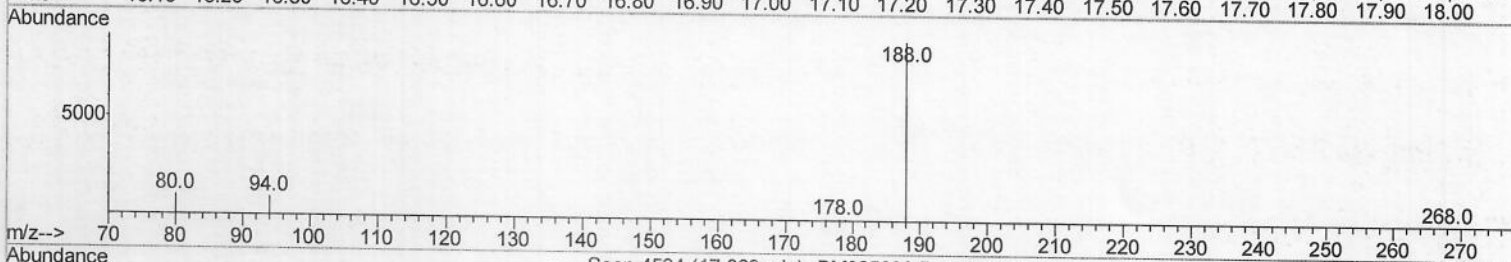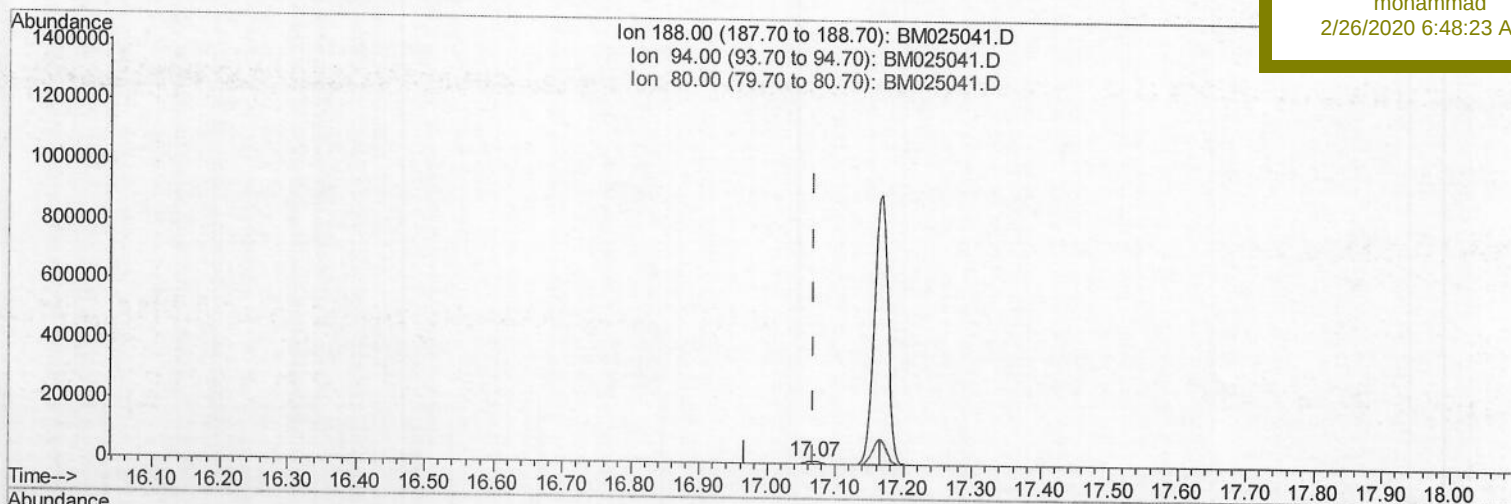Manual Integrations
APPROVEDmohammad
2/26/2020 6:48:23 AM

(10) Phenanthrene-d10 (I)

17.067min (-0.001) 0.40ng/ul m > JV 02126120

response 12558

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	10.69#
80.00	22.60	11.42#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
Data File : BM025041.D
Acq On : 25 Feb 2020 13:25
Operator : CG/JU
Sample : PB126774BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Feb 25 14:03:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK74

Manual Integrations
APPROVED

mohammad
2/26/2020 6:48:23 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	1929	0.40	ng/ul	0.00
2) Naphthalene-d8	10.47	136	8002	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.33	164	5528	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.07	188	12558m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	13253	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	14897	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	5907	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	16575	0.38	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SV 02/26/20