


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
Data File : BM025052.D
Acq On : 25 Feb 2020 20:04
Operator : CG/JU
Sample : L1486-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Feb 26 00:03:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBCX0

Manual Integrations
APPROVED

mohammad
2/26/2020 6:49:09 AM

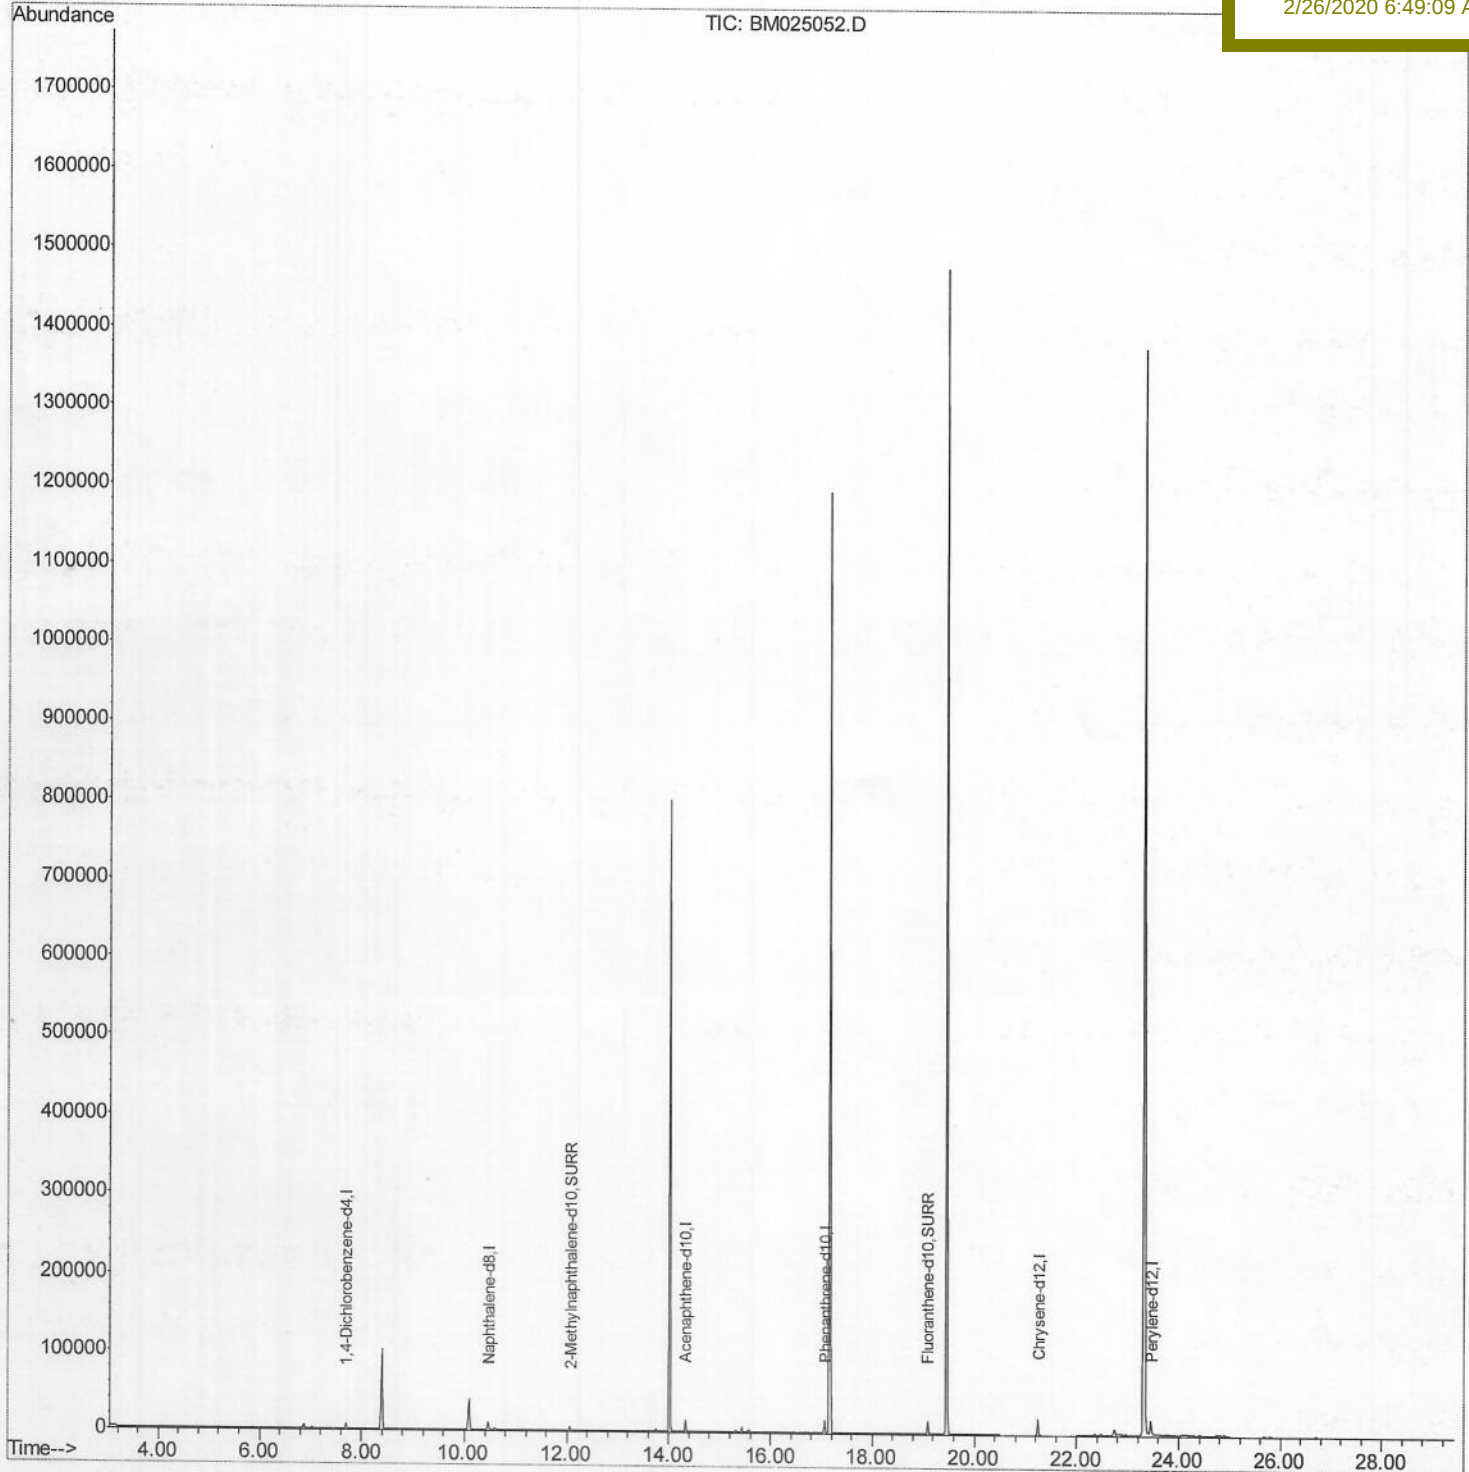

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025052.D

Acq On : 25 Feb 2020 20:04

Operator : CG/JU

Sample : L1486-18

Misc :

ALS Vial : 17 Sample Multiplier: 1

Quant Time: Feb 26 00:02:04 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBCX0

Manual Integrations

APPROVED

mohammad

2/26/2020 6:49:09 AM

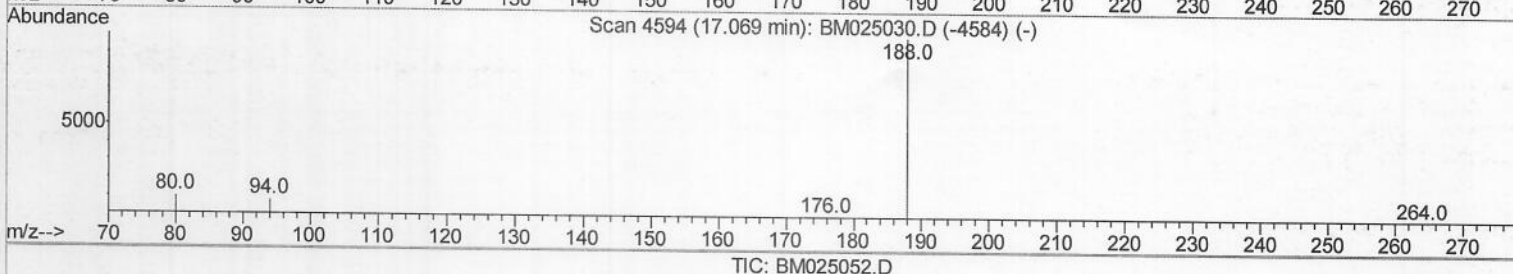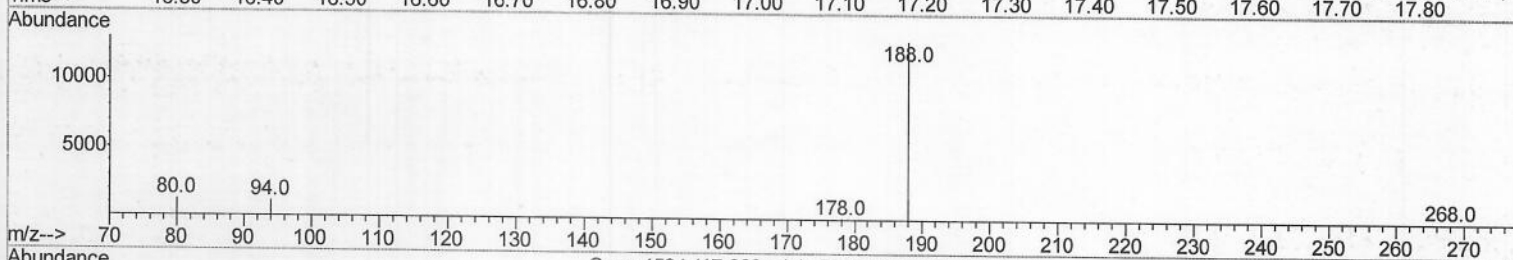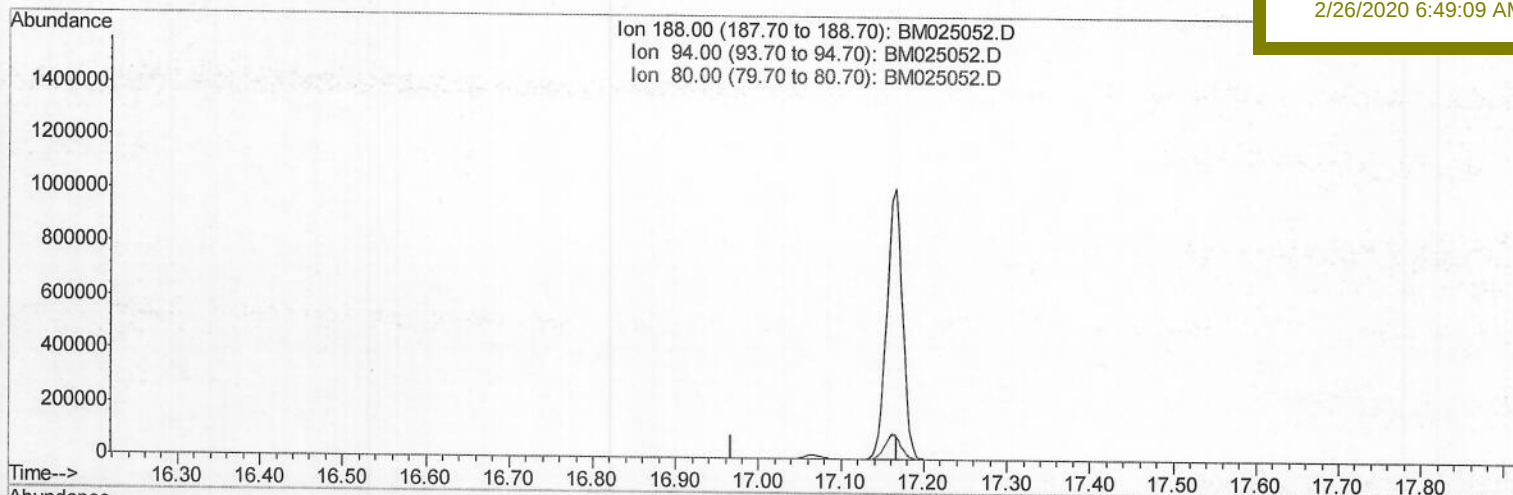

(10) Phenanthrene-d10 (I)

17.068min (-17.068) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025052.D

Acq On : 25 Feb 2020 20:04

Operator : CG/JU

Sample : L1486-18

Misc :

ALS Vial : 17 Sample Multiplier: 1

Quant Time: Feb 26 00:02:04 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

DBCX0

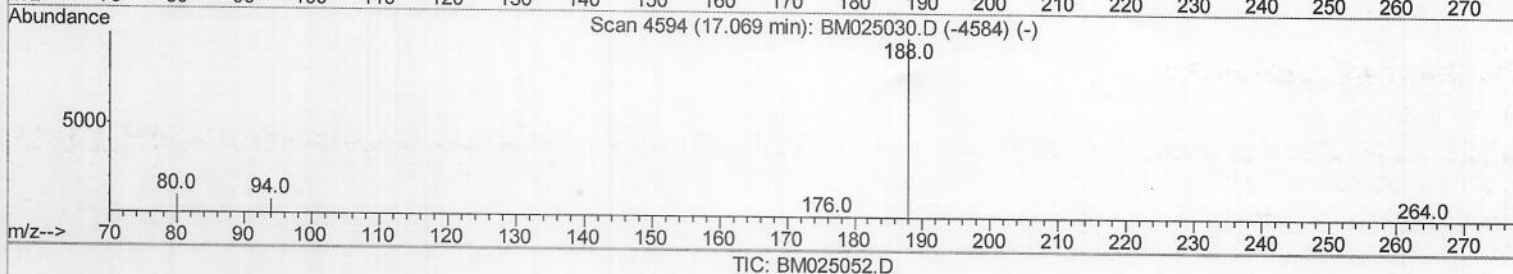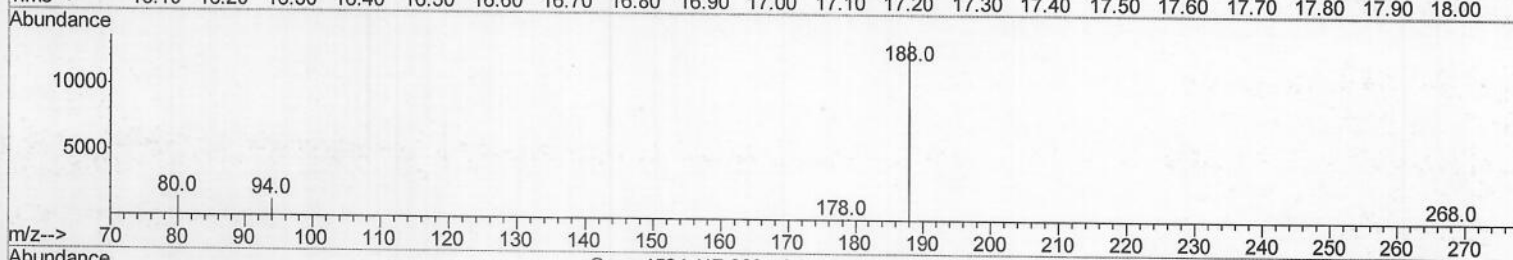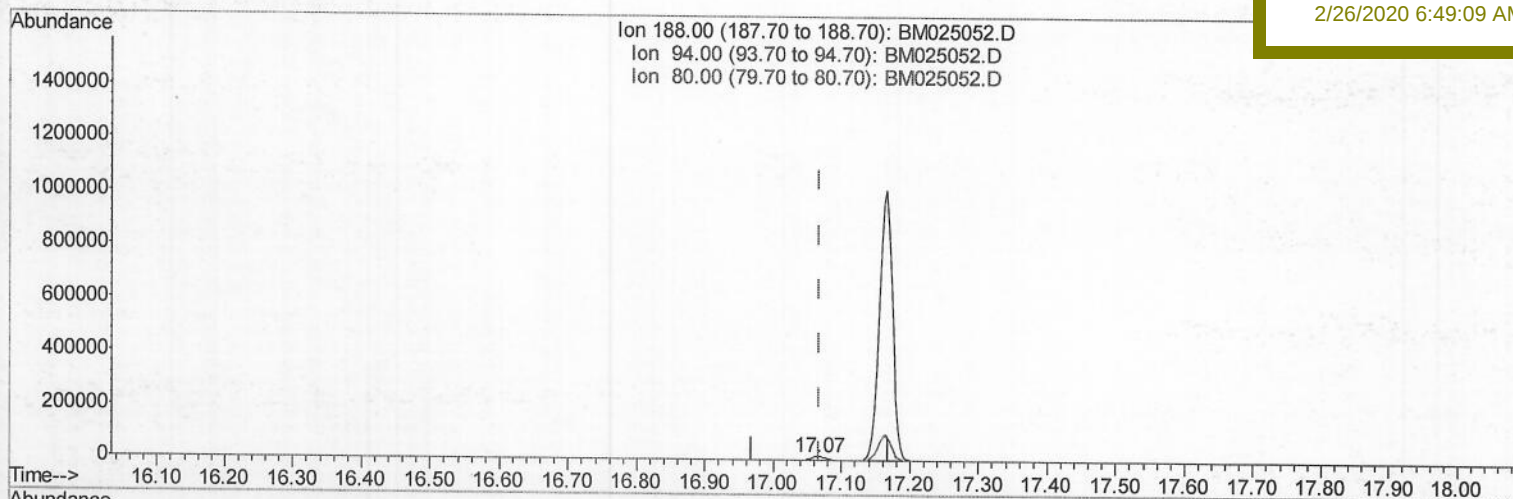Manual Integrations
APPROVEDmohammad
2/26/2020 6:49:09 AM

(10) Phenanthrene-d10 (I)

17.065min (-0.003) 0.40ng/ul m>SV 02/26/20

response 18166

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	9.44#
80.00	22.60	10.46#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
 Data File : BM025052.D
 Acq On : 25 Feb 2020 20:04
 Operator : CG/JU
 Sample : L1486-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBCX0

Quant Time: Feb 26 00:03:21 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 25 11:03:43 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 2/26/2020 6:49:09 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	3178	0.40	ng/ul	0.00
2) Naphthalene-d8	10.47	136	12651	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.33	164	8186	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.07	188	18166m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	19228	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	22751	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	6250	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	17300	0.28	ng/ul	0.00

SV 02/26/20

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed