

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025054.D

Acq On : 25 Feb 2020 21:16

Operator : CG/JU

Sample : L1486-21

Misc :

ALS Vial : 19 Sample Multiplier: 1

Quant Time: Feb 26 00:07:11 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :


DBCX3

Manual Integrations

APPROVED

mohammad

2/26/2020 6:49:19 AM

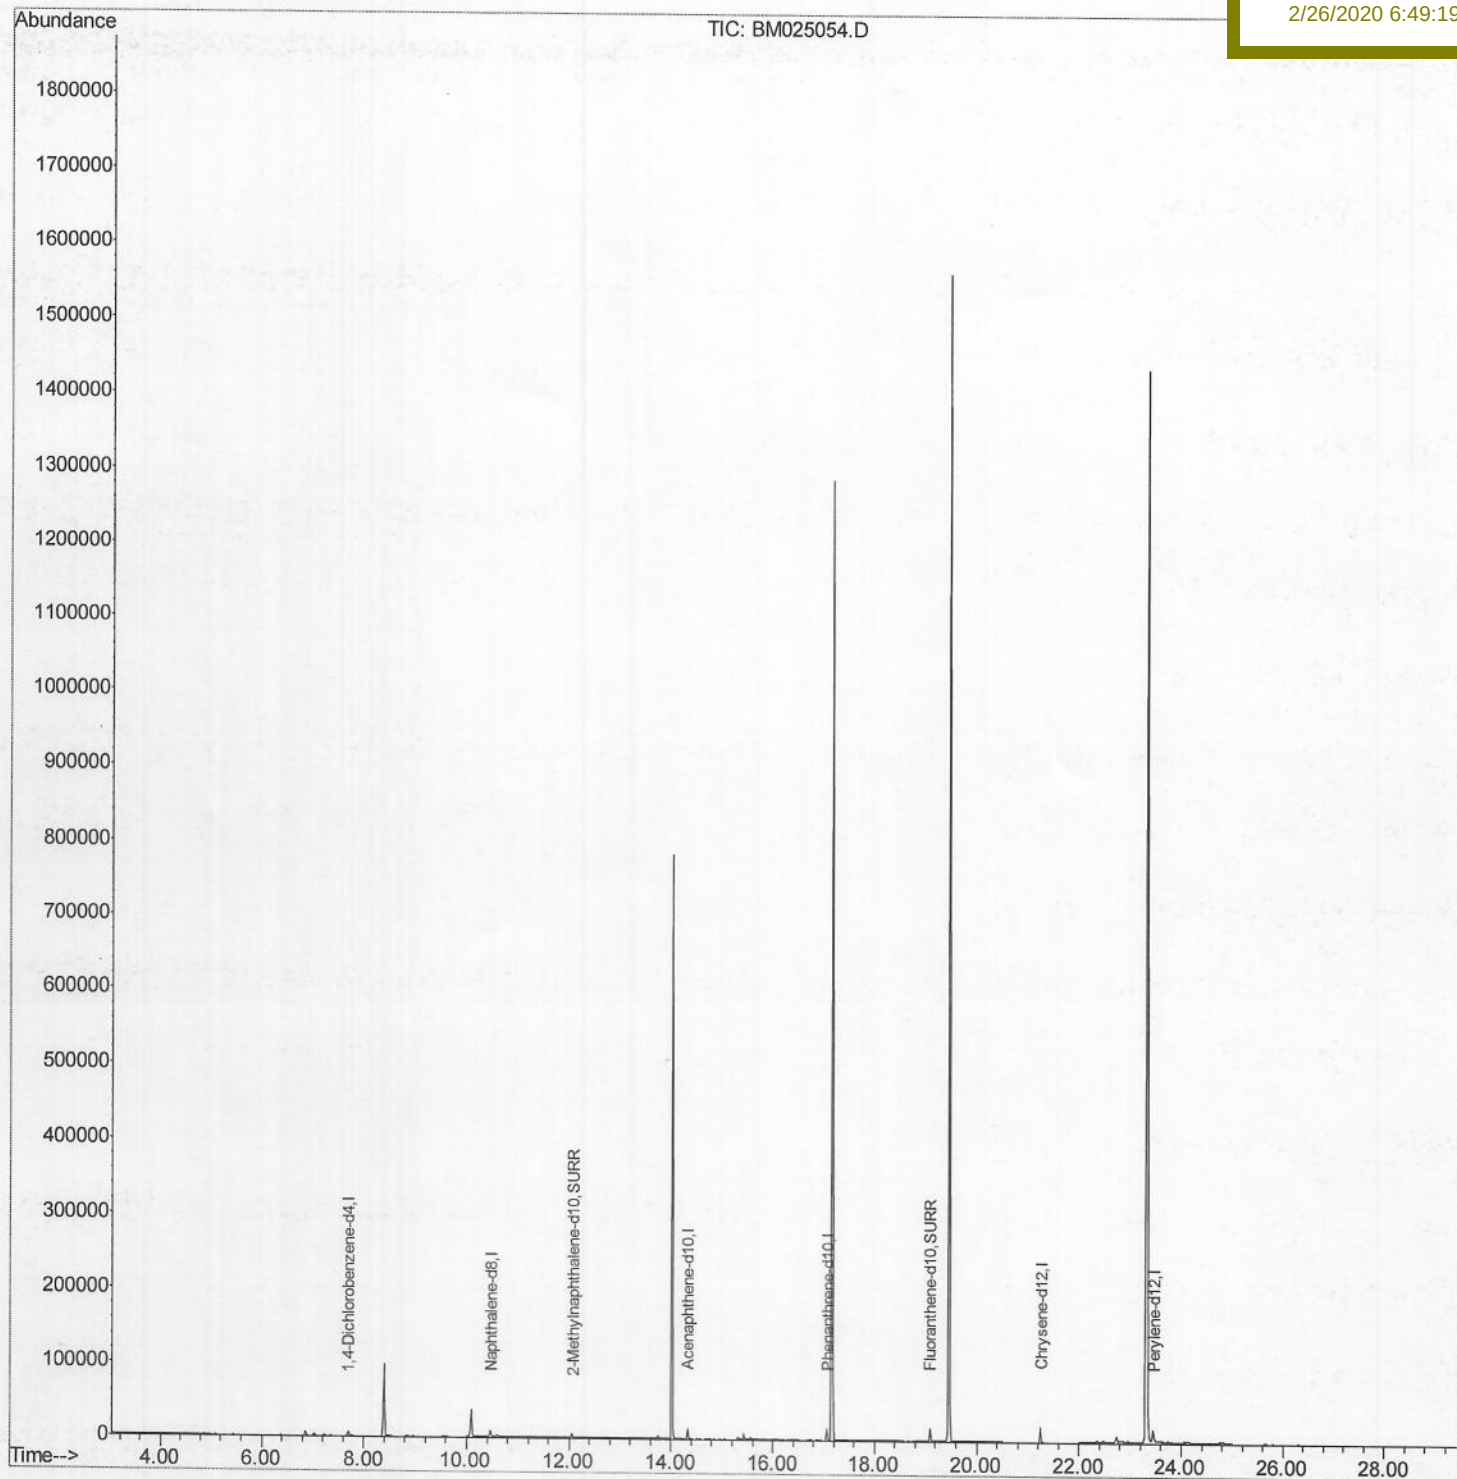

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025054.D

Acq On : 25 Feb 2020 21:16

Operator : CG/JU

Sample : L1486-21

Misc :

ALS Vial : 19 Sample Multiplier: 1

Quant Time: Feb 26 00:06:01 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBCX3

Manual Integrations

APPROVED

mohammad

2/26/2020 6:49:19 AM

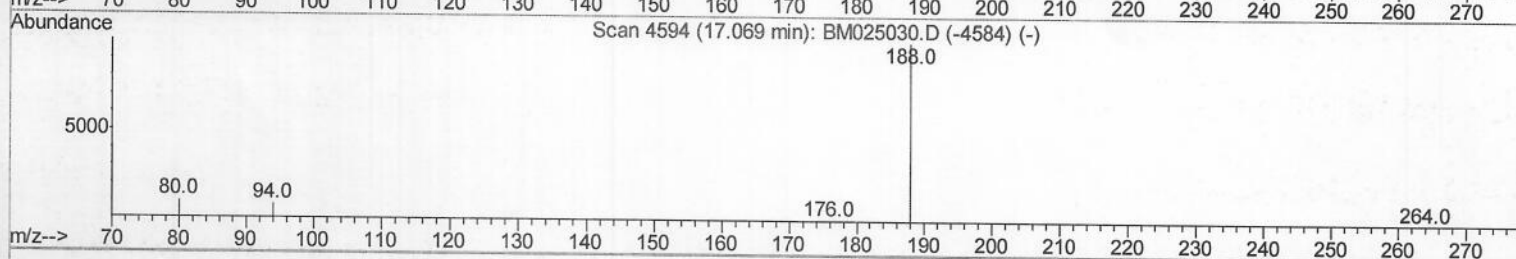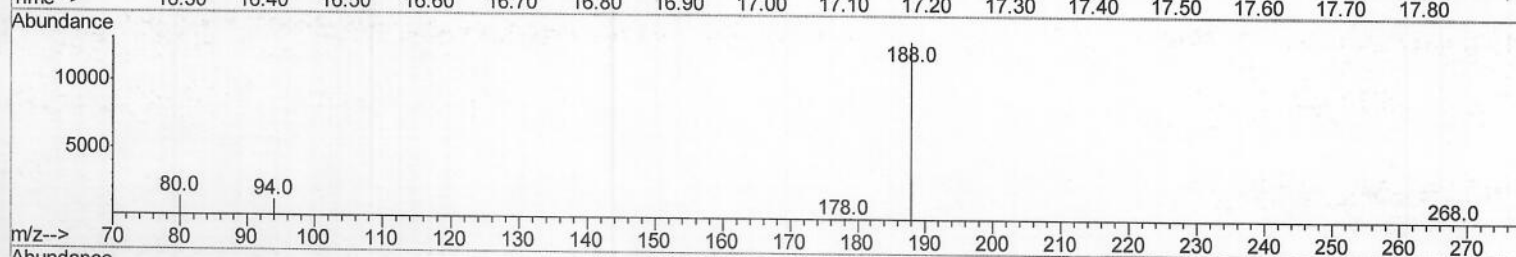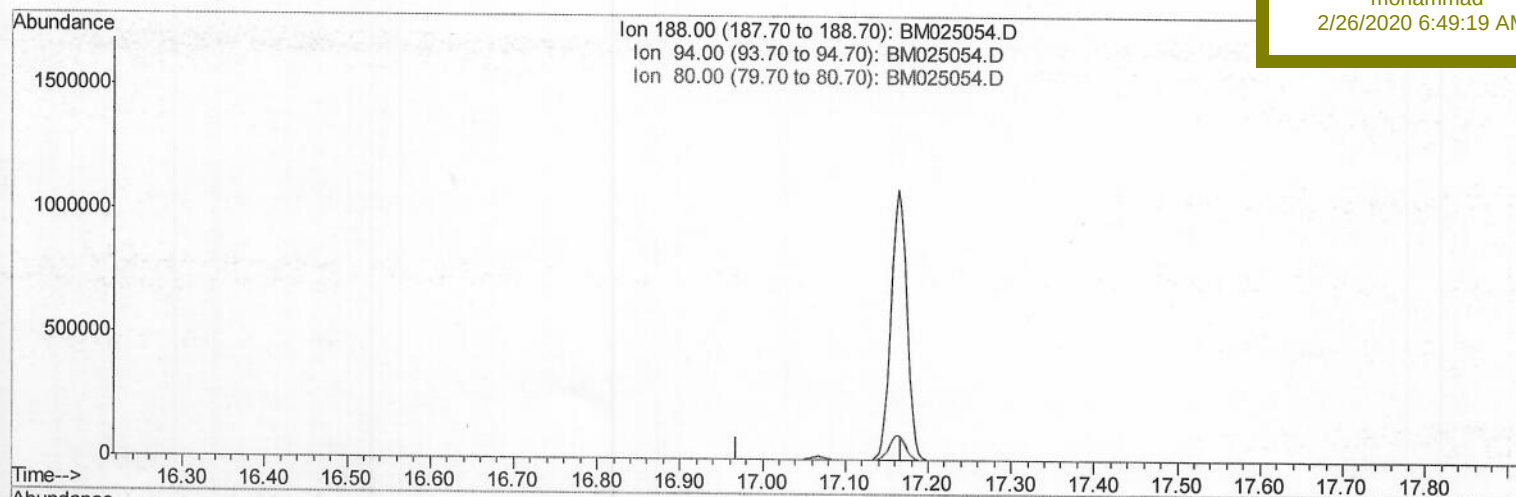

TIC: BM025054.D

(10) Phenanthrene-d10 (I)

17.068min (-17.068) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025054.D

Acq On : 25 Feb 2020 21:16

Operator : CG/JU

Sample : L1486-21

Misc :

ALS Vial : 19 Sample Multiplier: 1

Quant Time: Feb 26 00:06:01 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBCX3

Manual Integrations

APPROVED

mohammad

2/26/2020 6:49:19 AM

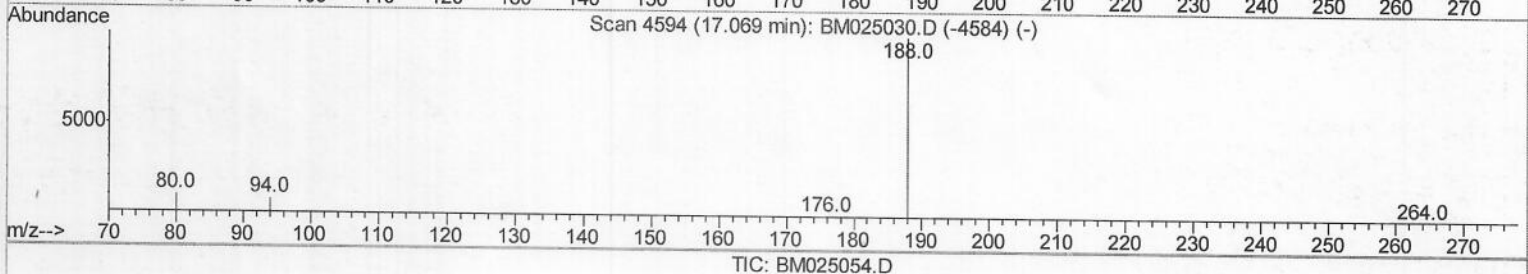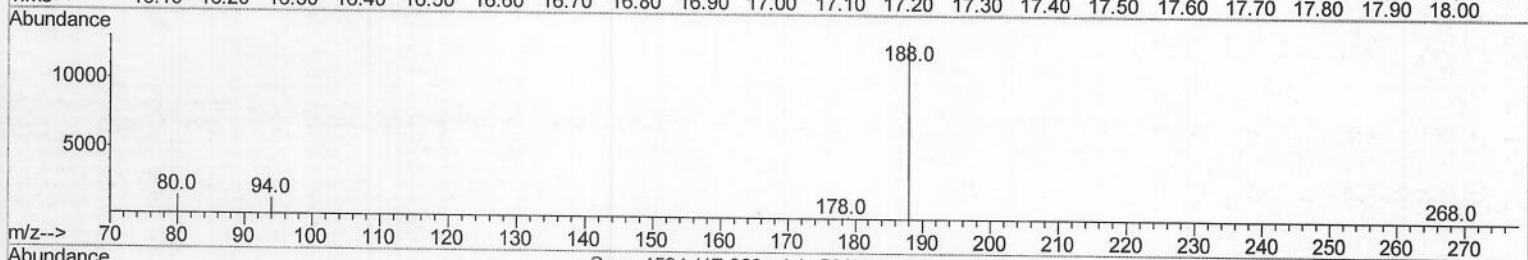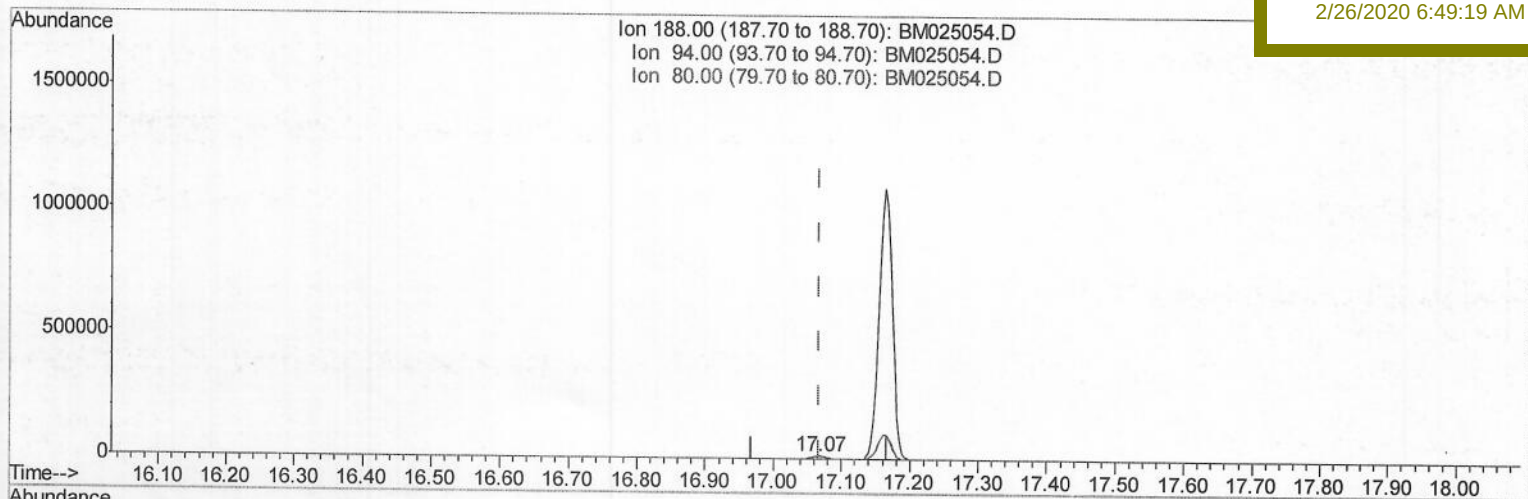

(10) Phenanthrene-d10 (I)

17.067min (-0.001) 0.40ng/ul m > JV 02/26/20

response 17627

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	9.16#
80.00	22.60	10.37#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
Data File : BM025054.D
Acq On : 25 Feb 2020 21:16
Operator : CG/JU
Sample : L1486-21
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Feb 26 00:07:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :
BNA_M
Client Sampled :
DBCX3

Manual Integrations
APPROVED

mohammad
2/26/2020 6:49:19 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	3125	0.40	ng/ul	0.00
2) Naphthalene-d8	10.47	136	12195	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.32	164	7936	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.07	188	17627m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	18214	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	20533	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	5941	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	18524	0.31	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed