


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022520\
Data File : BM025060.D
Acq On : 26 Feb 2020 01:29
Operator : CG/JU
Sample : PB126855BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Feb 29 02:36:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

mohammad
2/27/2020 4:59:33 PM

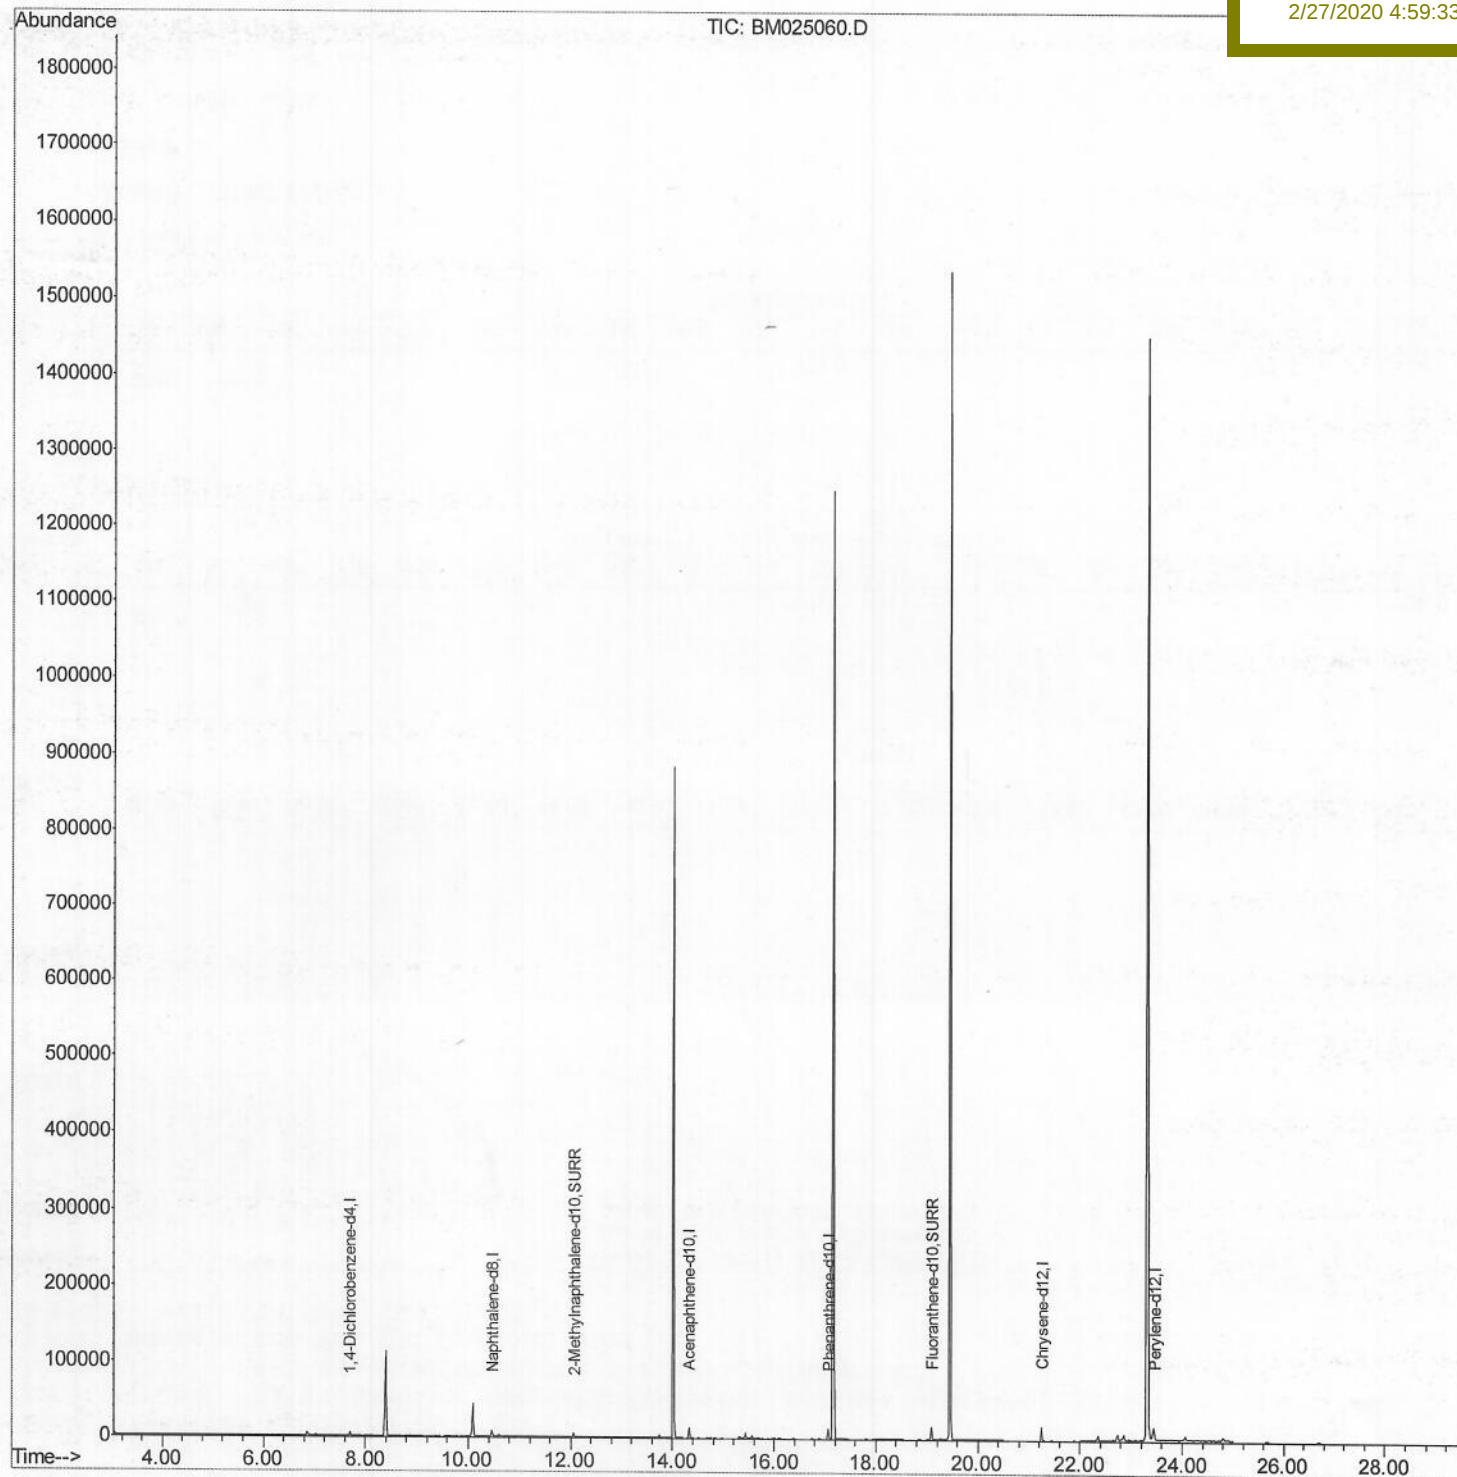

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025060.D

Acq On : 26 Feb 2020 01:29

Operator : CG/JU

Sample : PB126855BL

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Feb 26 03:36:31 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




SBLK55

Manual Integrations

APPROVED

mohammad

2/27/2020 4:59:33 PM

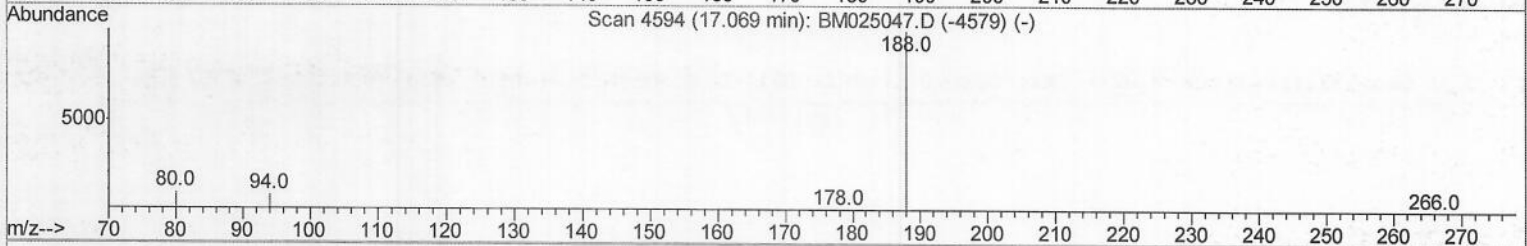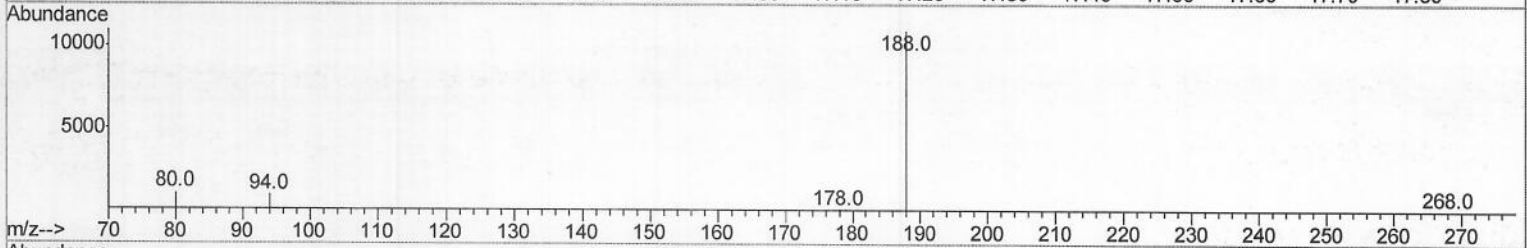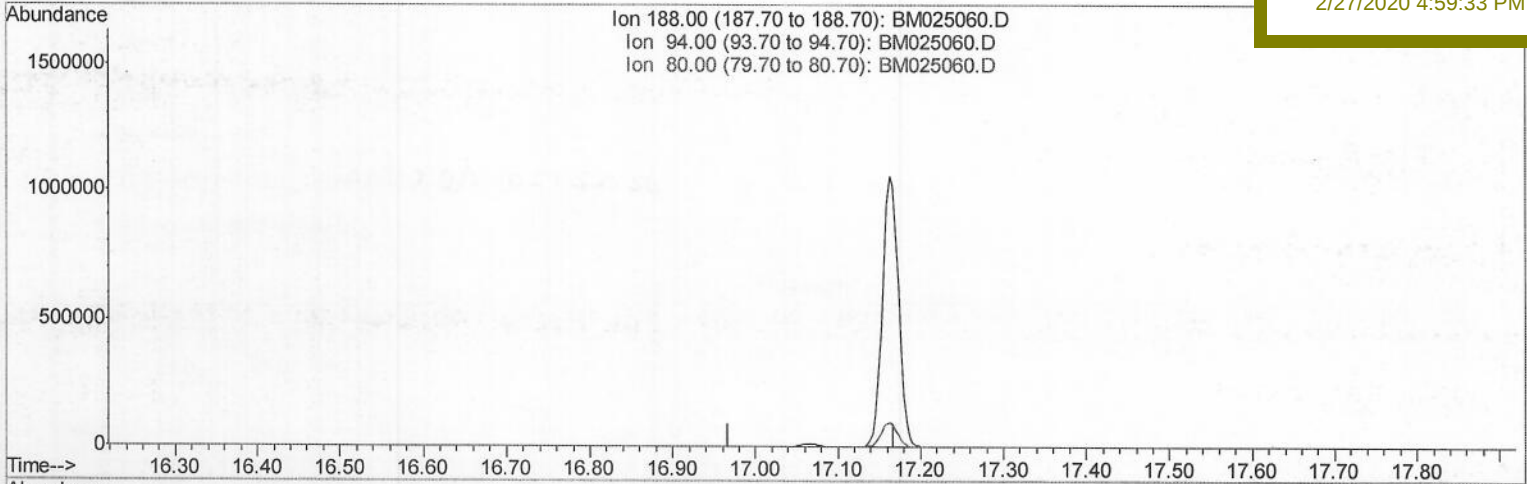

TIC: BM025060.D

(10) Phenanthrene-d10 (I)

17.068min (-17.068) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025060.D

Acq On : 26 Feb 2020 01:29

Operator : CG/JU

Sample : PB126855BL

Misc :

ALS Vial : 24 Sample Multiplier: 1

Quant Time: Feb 26 03:36:31 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




SBLK55

Manual Integrations

APPROVED

mohammad

2/27/2020 4:59:33 PM

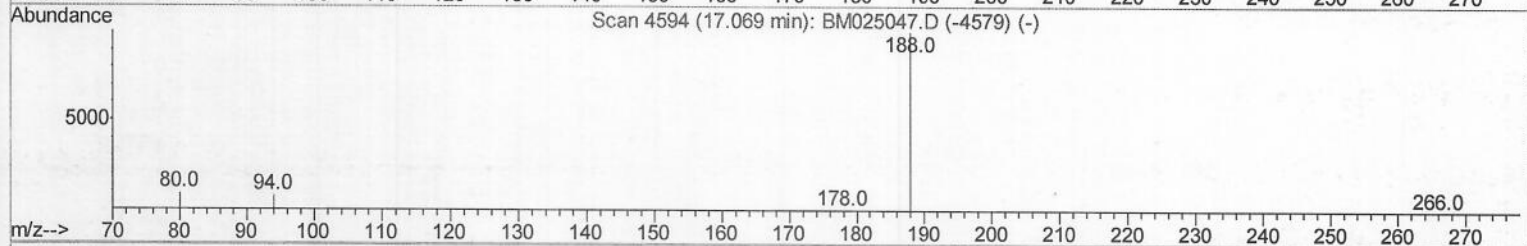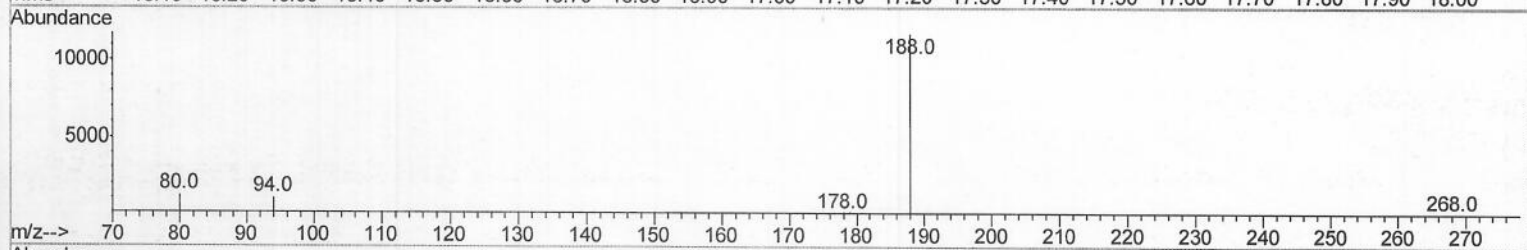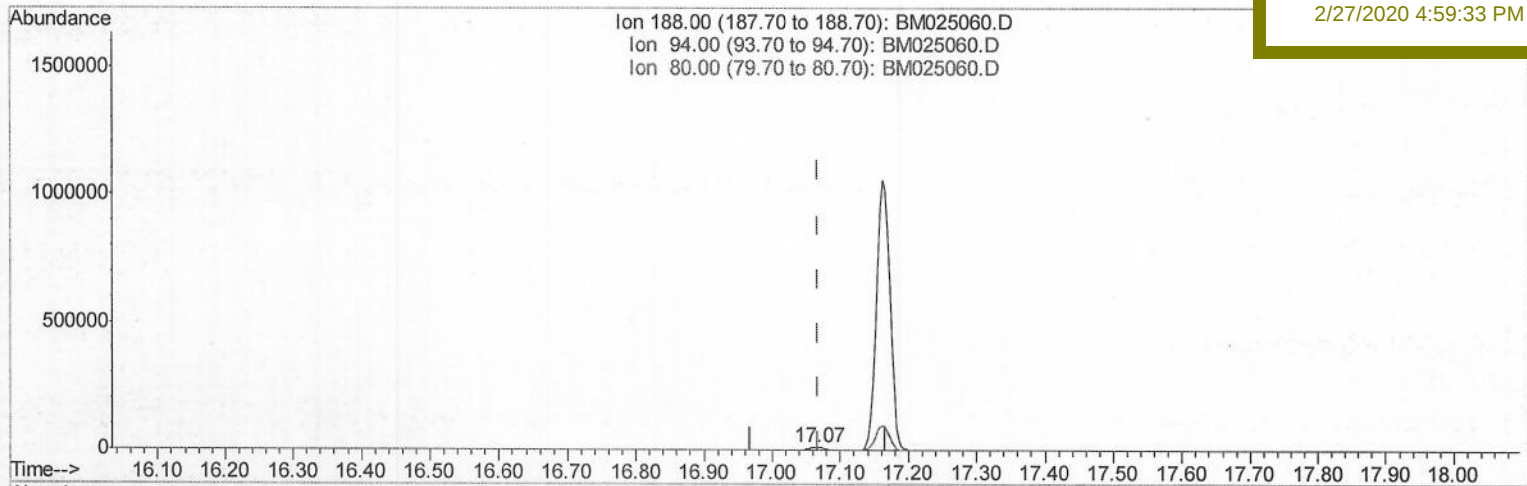

TIC: BM025060.D

(10) Phenanthrene-d10 (I)

17.065min (-0.003) 0.40ng/ul m>JU 02/27/20

response 15961

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	8.77#
80.00	22.60	10.03#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022520\
Data File : BM025060.D
Acq On : 26 Feb 2020 01:29
Operator : CG/JU
Sample : PB126855BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Feb 29 02:36:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

mohammad
2/27/2020 4:59:33 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	2782	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	10928	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.32	164	7150	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.07	188	15961m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	16842	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	20265	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	6802	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	18402	0.34	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed