


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
Data File : BM025062.D
Acq On : 26 Feb 2020 02:41
Operator : CG/JU
Sample : PB126903BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Feb 26 11:24:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampled :
SBLK03

Manual Integrations
APPROVED

mohammad
2/27/2020 4:59:39 PM

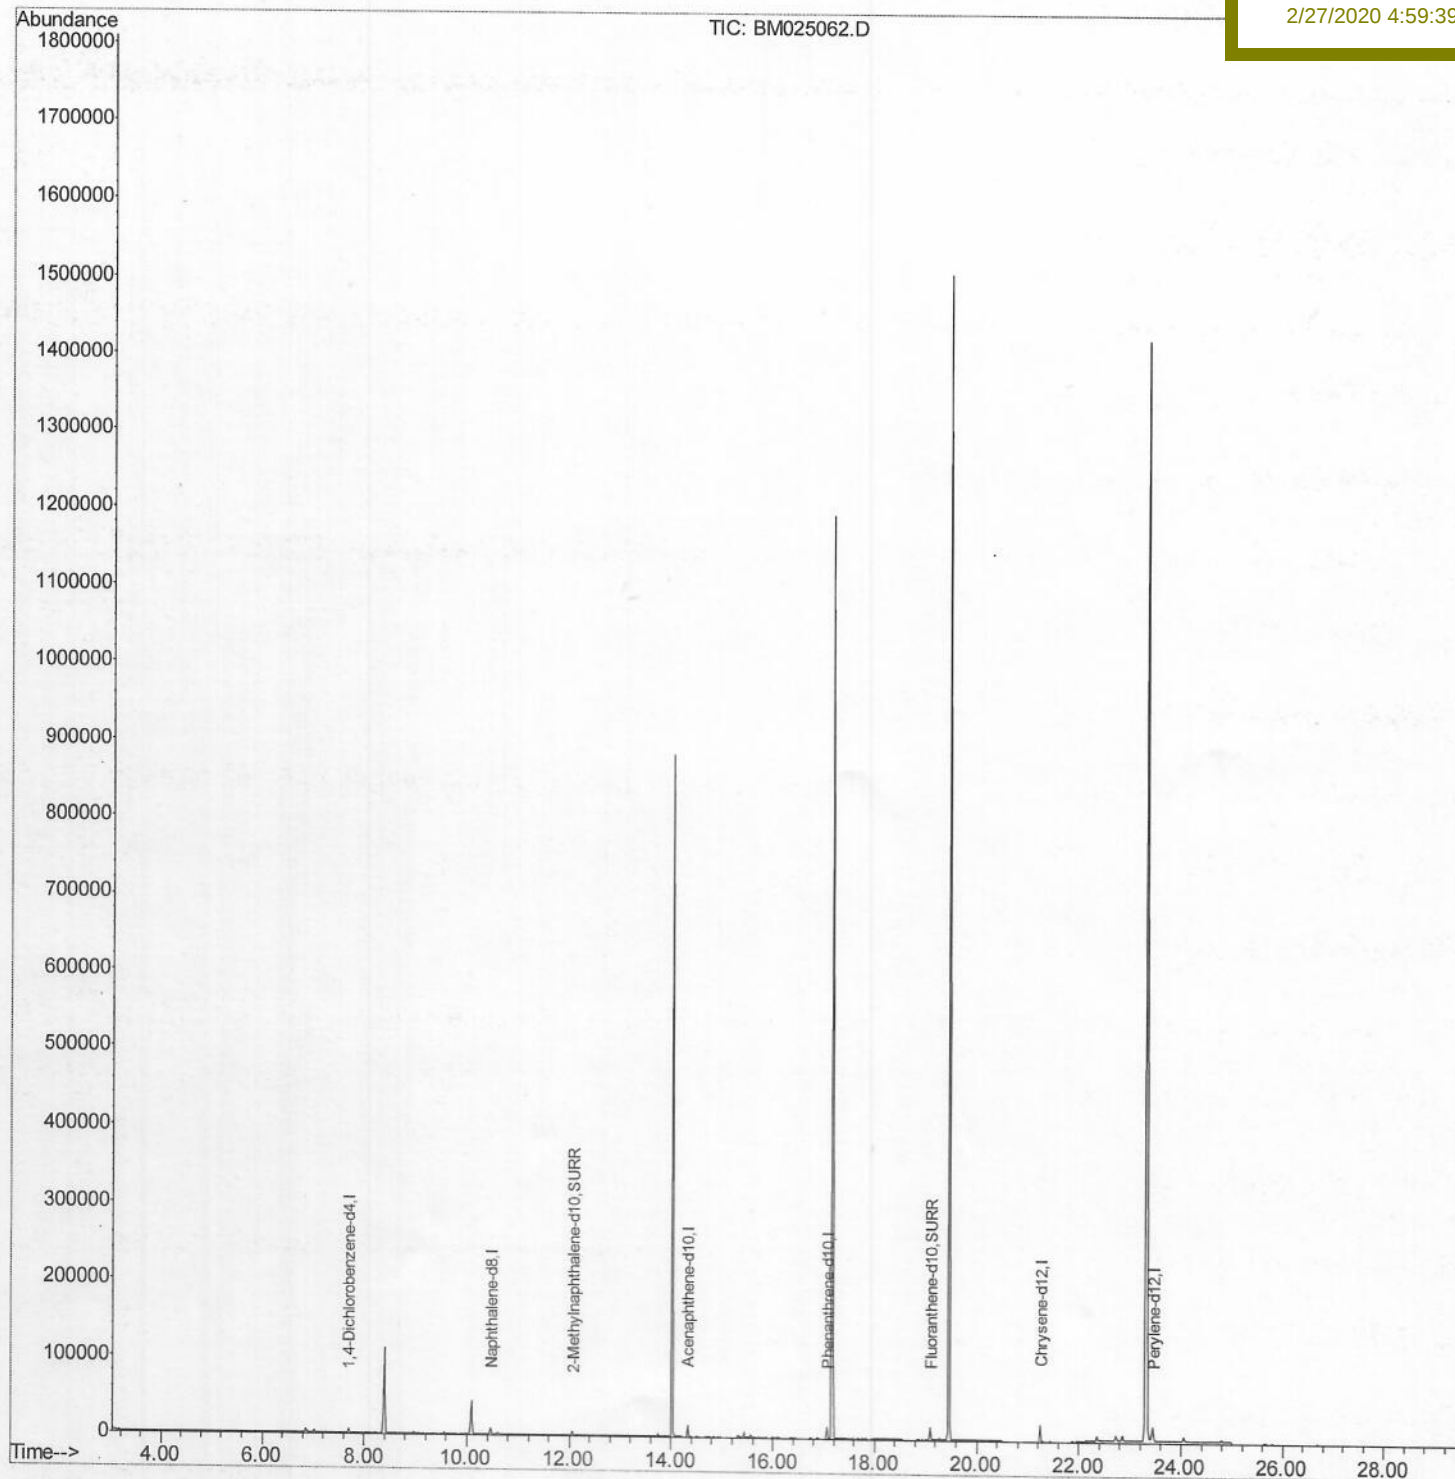

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
 Data File : BM025062.D
 Acq On : 26 Feb 2020 02:41
 Operator : CG/JU
 Sample : PB126903BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Quant Time: Feb 26 11:23:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 25 11:03:43 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 SBLK03

Manual Integrations
 APPROVED

mohammad
 2/27/2020 4:59:39 PM

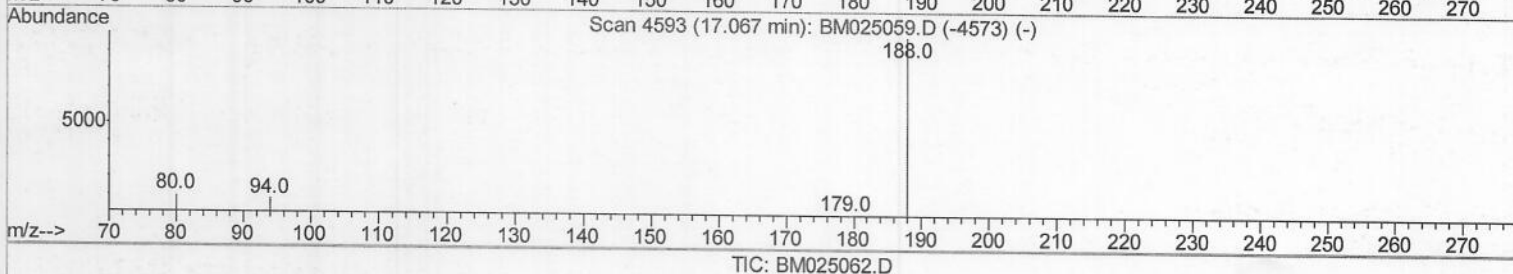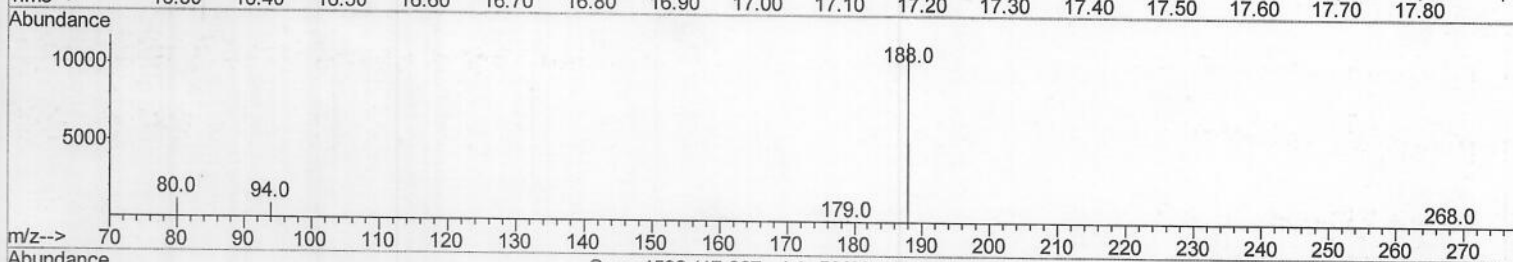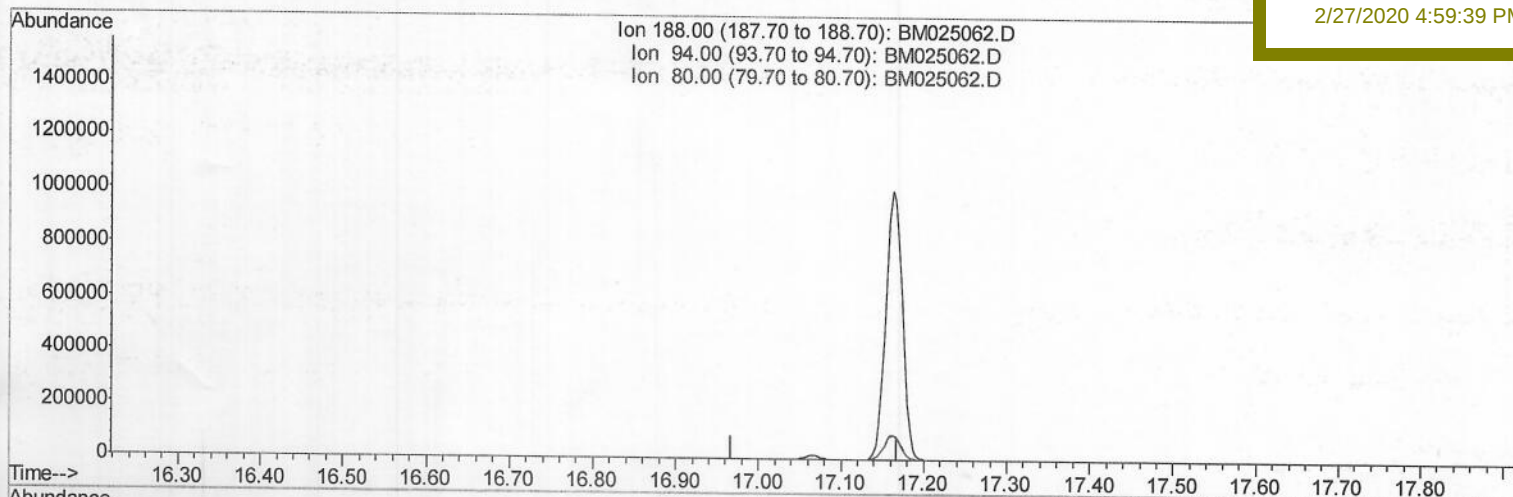

TIC: BM025062.D

(10) Phenanthrene-d10 (I)

17.068min (-17.068) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025062.D

Acq On : 26 Feb 2020 02:41

Operator : CG/JU

Sample : PB126903BL

Misc :

ALS Vial : 26 Sample Multiplier: 1

Quant Time: Feb 26 11:23:42 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

SBLK03

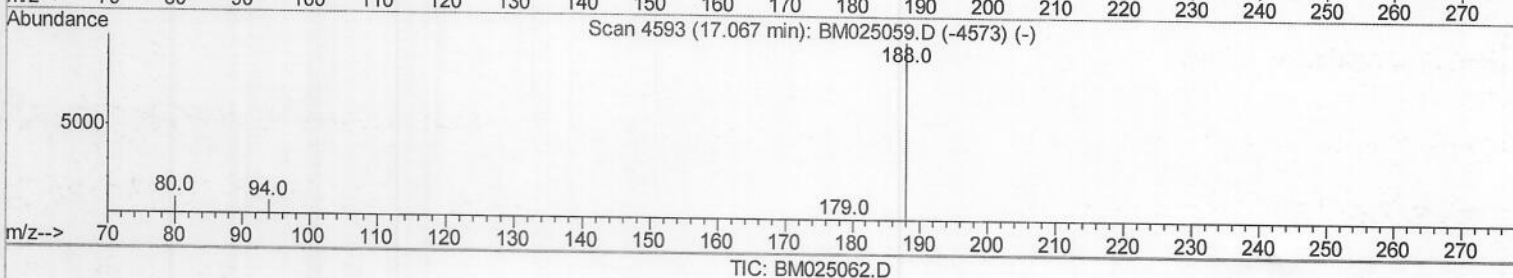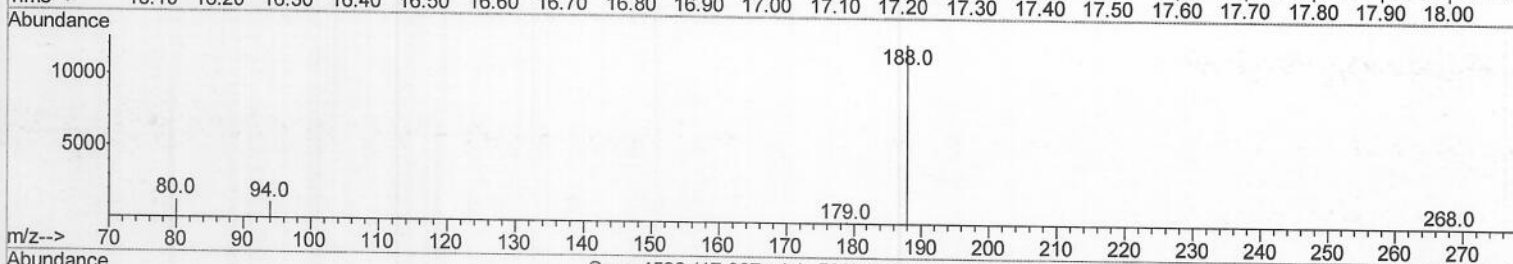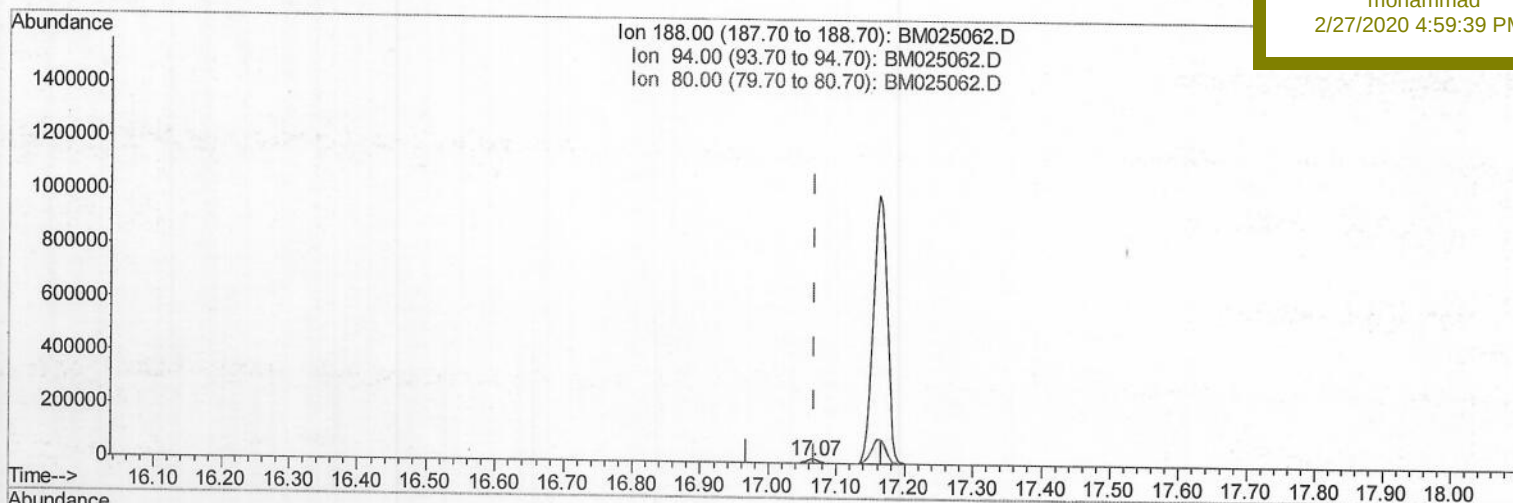Manual Integrations
APPROVEDmohammad
2/27/2020 4:59:39 PM

(10) Phenanthrene-d10 (I)

17.065min (-0.003) 0.40ng/ul m *JU 02/27/20*

response 17236

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	9.06#
80.00	22.60	10.28#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
Data File : BM025062.D
Acq On : 26 Feb 2020 02:41
Operator : CG/JU
Sample : PB126903BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Feb 26 11:24:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :
BNA_M
Client Sampled :
SBLK03

Manual Integrations
APPROVED

mohammad
2/27/2020 4:59:39 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	2968	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	11744	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.32	164	7625	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.07	188	17236m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	18169	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	21568	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	6773	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	18187	0.31	ng/ul	0.00

Target Compounds

					Ovalue
--	--	--	--	--	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 02/27/20